ENDEVCO

MODEL 2775A
SIGNAL CONDITIONER

INSTRUCTION MANUAL

ENDEVCO

San Juan Capistrano, California, U.S.A.

IM2775A
Revision U
September 21, 1992

Digitized by the Internet Archive
in 2025

https://archive.org/details/manualsplus_10636

TABLE OF CONTENTS

SECTION 1:	DESCRIPTION	PAGE
1.	EQUIPMENT DESCRIPTION	1-1
2.	EQUIPMENT USE	1-3
SECTION 2:	**CONTROLS, CONNECTORS AND OPERATING INSTRUCTIONS**	
1.	INTRODUCTION	2-1
2.	FRONT PANEL CONTROLS	2-1
3	REAR PANEL CONTROLS	2-5
4.	INTERNAL CONTROLS	2-6
SECTION 3:	**INSTALLATION AND CHECKOUT**	
1.	UNPACKING AND INSPECTION	3-1
2.	INSTALLATION	3-1
3.	CHECKOUT	3-2
4.	OPERATION	3-4
SECTION 4:	**THEORY OF OPERATION, CIRCUIT DESCRIPTION AND SPECIFICATIONS**	
1.	THEORY OF OPERATION	4-1
2.	CIRCUIT DESCRIPTION	4-3
3.	SPECIFICATIONS	4-8
SECTION 5:	**MAINTENANCE AND CALIBRATION**	
1.	MAINTENANCE	5-1
2.	CALIBRATION	5-1
3.	INITIAL SETUP	5-2
4.	OUTPUT CAL	5-4
5.	COMMON MODE VOLTAGE	5-5
6.	TEST INPUT	5-6
7.	EXTERNAL CAL INPUT	5-6
8.	MAX I OUT	5-6
9.	NOISE	5-7
10	GAIN ACCURACY	5-7
11.	SENSITIVITY SWITCH TEST	5-9
12.	FREQUENCY RESPONSE	5-9
13.	REMOTE GAIN ACCURACY	5-10
14.	REMOTE FREQUENCY RESPONSE	5-11

TABLE OF CONTENTS

SECTION 5:	MAINTENANCE AND CALIBRATION (continued)	PAGE
15.	REMOTE NOISE	5-11
16.	CONSTANT CURRENT ADJUST	5-12
17.	TROUBLESHOOTING GUIDE	5-12
18.	REPAIR	5-14
19.	FACTORY SERVICE	5-14
SECTION 6	**OPTIONS AND ACCESSORIES**	
1.	ACCESSORIES INCLUDED	6-1
2.	ACCESSORIES AVAILABLE	6-1
3.	ADJUSTABLE FILTER	6-2
4.	REMOTE CHARGE CONVERTER	6-5
SECTION 7	**DRAWINGS AND PARTS LISTS**	
1.	GENERAL	7-1
2.	PARTS LISTS	7-1
3.	DRAWINGS	7-1

FIGURES

1-1	MODEL 2775A SIGNAL CONDITIONER	1-1
2-1	MODEL 2775A FRONT PANEL	2-1
2-2	SENSITIVITY AND FULL SCALE SELECTION	2-2
2-3	REAR PANEL CONTROLS AND CONNECTORS	2-5
2-4	INTERNAL CONTROLS	2-6
3-1	IINTERNAL CONTROLS	3-1
3-2	FRONT PANEL CONTROLS	3-3
3-3	OUTPUT CALIBRATION	3-3
3-4	EXTERNAL CALIBRATION INPUT	3-4
3-5	TEST INPUT	3-7
3-6	REMOTE TRANSFER	3-11
3-7	REMOTE HOOKUP	3-12
3-8	FREQUENCY RESPONSE NOMOGRAPH	3-12
4-1	SiIMPLIFIED EQUIVALENT CIRCUIT	4-1

TABLE OF CONTENTS

FIGURES (continued)		PAGE
4-2	CHARGE CONVERTER CIRCUIT	4-2
4-3	MODEL 2775 BLOCK	4-3
5-1	FRONT PANEL CONTROLS	5-2
5-2	REAR PANEL CONTROLS	5-2
5-3	INTERNAL CONTROLS	5-3
5-4	POWER SUPPLY TEST POINTS	5-4
5-5	OOUTPUT CALIBRATION	5-5
5-6	COMMON MODE	5-5
5-7	TEST INPUT	5-6
5-8	EXTERNAL CALIBRATION	5-6
5-9	NOISE	5-7
5-10	GAIN ACCURACY	5-8
5-11	FREQUENCY RESPONSE	5-10
5-12	REMOTE GAIN	5-10
5-13	REMOTE NOISE	5-12
5-14	CONSTANT CURRENT ADJUST	5-12
6-1	PROGRAMMING JUMPER SELECTION	6-3
6-2	CUT-OFF RESISTOR POSITIONS	6-3
6-3	HIGH-PASS FILTER RESISTOR SELECTION CHART	6-4
6-4	LOW-PASS FILTER RESISTOR SELECTION CHART	6-5
6-5	2771A DIMENSIONS	6-6
6-6	2771A/2775A TEST SETUP	6-7
6-7	2771A GIAN AND BIAS SETUP	6-8

TABLES		
2-1	SENSITIVITY AND FULL SCALE RANGE SELECTION	2-2
2-2	CALCULATION OF mV/g VALUES	2-3
4-1	2775A MEMORY MAP	4-4
4-2	VOLTAGE AMPLIFIER GAIN	4-7
4-3	SERVO AMPLIFIER GAIN CONTROLS	4-7

SECTION 1
DESCRIPTION

1. EQUIPMENT DESCRIPTION

The ENDEVCO Model 2775A Signal Conditioner is a solid-state instrument designed to condition either the low-level analog acceleration signals from a piezoelectric (PE) transducer or the amplified signals from an Isotron transducer or a remote charge converter. The outputs are AC, DC, and SERVO signals proportional to the acceleration input signal. A back panel switch on the conditioner selects the charge converter stage for direct PE transducer input connection or a constant current signal conditioning stage for accepting the input from a remote preamp device. This flexibility broadens the transducer choices which can be used.

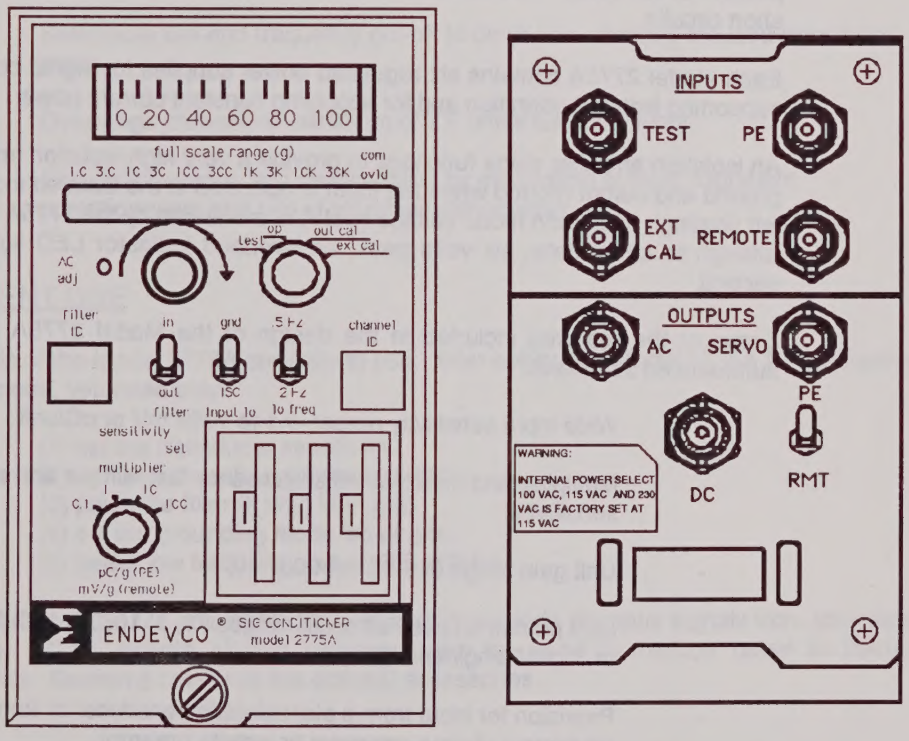

FIGURE 1-1. MODEL 2775A SIGNAL CONDITIONER

When the charge converter stage is switched in, the transducer sensitivity and transducer frequency response are independent of the cable length between the transducer and signal conditioner. Low frequency response of the signal conditioner is also independent of transducer and cable capacitance and depends only on the selected low frequency response of the charge converter

For applications where pre-conditioning of the signal is necessary, the Model 2775A can accept the input signal from a remote preamp device. When operating in this mode, the 2775A supplies the constant bias current necessary to operate a compatible remote preamp device such as an Isotron transducer or remote charge converter. This mode of operation is better suited where low resistance transducers, electrical noise, or long leads from remote locations can affect the acquisition of data.

Data signals are processed and normalized as three independent outputs. First is an AC output which is front panel adjustable from 1 to 10 V pk full scale. The AC output has 85 mA capability sufficient to drive most galvonometer or capacitive loads. A second output is a servo signal scaled for 10mV/g or 100mV/g depending on the placement of an internally inserted jumper clip, factory set to 10mV/g. The third output is a DC signal which provides a linear low impedance output proportional to signal average which is normalized to 10 V dc full scale for driving strip chart recorders, etc. The panel meter is driven by the DC output, displaying a linear scale in percent of full scale. All outputs are buffered and current limited to protect against accidental short circuits.

Each Model 2775A contains six regulated power supplies for signal conditioner operation, for supporting isolated operation and for supplying constant current power.

An isolation amplifier stage functions to provide a very high isolation impedance between input ground and output ground when the input is operated in the isolated mode (i.e., input ground is left floating). Common mode voltage (CMV) is monitored by the 2775A. When the CMV is high enough to affect data, six volts peak, an overload indicator LED lights up for at least one second.

Some of the features included in the design of the Model 2775A Signal Conditioner are summarized as follows:

- Wide input sensitivity range: 0.1 to 1099 mV or pC/unit.
- Multiplier and thumbwheel switches for fast, simple and exact entry of transducer sensitivity.
- Unit gain range of 0.03 to 1000.
- LED pointer shows Full scale ranges: 1, 3, 10, 30, 100, 300, 1000, 3000, 10,000 or 30,000 engineering units.
- Provision for input from a piezoelectric transducer or from an Isotron transducer (or remote charge converter or remote preamp).
- Provision for operating the input in a grounded or isolated (floating) mode.
- High impedance (50 M ohms minimum) isolation between input common and output common grounds in the isolated mode.
- Common-mode overload LED for announcing the detection of an excessive common-mode-voltage.
- In-out filter control of an optional Model 35771 selectable filter: high-pass, low-pass or bandpass filtration of data signals.

- Test input for an external test signal to check the integrity of transducer and signal conditioner operation.
- Output calibration oscillator generates a precise full scale signal for calibration of measuring and recording devices.
- External calibration input for functional calibration check of the signal conditioner.
- Operates from 100-, 115-, or 230-volts, 50-400 Hz.
- Single-channel, stand alone, operation or six-channel operation in a Model 4948 19-inch rack adapter.
- Buffered outputs current limited for short-circuit protection.
- Selectable low-end frequency cut-off to block non-vibratory induced transducer noise.
- Overrange protection: minimum of 7.5 times full scale input.
- Easy maintenance and serviceability by elimination of most alignment potentiometers and use of standard components.

2. EQUIPMENT USE

The controls of the Model 2775A are easy to use. After setting the Model 2775A for the desired operating mode, you need only:

(1) set the transducer sensitivity.
(2) set the full scale engineering units.
(3) place the filter (if any) in or out.
(4) set the grounding mode iso or gnd.
(5) select low frequency cut-off 0.5 or 2 Hz.

The optional Model 35771 adjustable filter will help to exclude spurious signals from your data. The Model 2771A remote charge converter can be used to reduce noise in hostile environments. Section 6 covers all the optional accessories.

SECTION 2
CONTROLS AND CONNECTORS

1. INTRODUCTION

The Model 2775A front panel has seven control switches and one output adjustment pot. The back panel has one input mode switch, four input connectors, and three output connectors. Internally, on the main circuit board, the unit has a input power switch, fuse holder, servo range jumper, constant current pot, and two common mode adjust pots.

2. FRONT PANEL CONTROLS

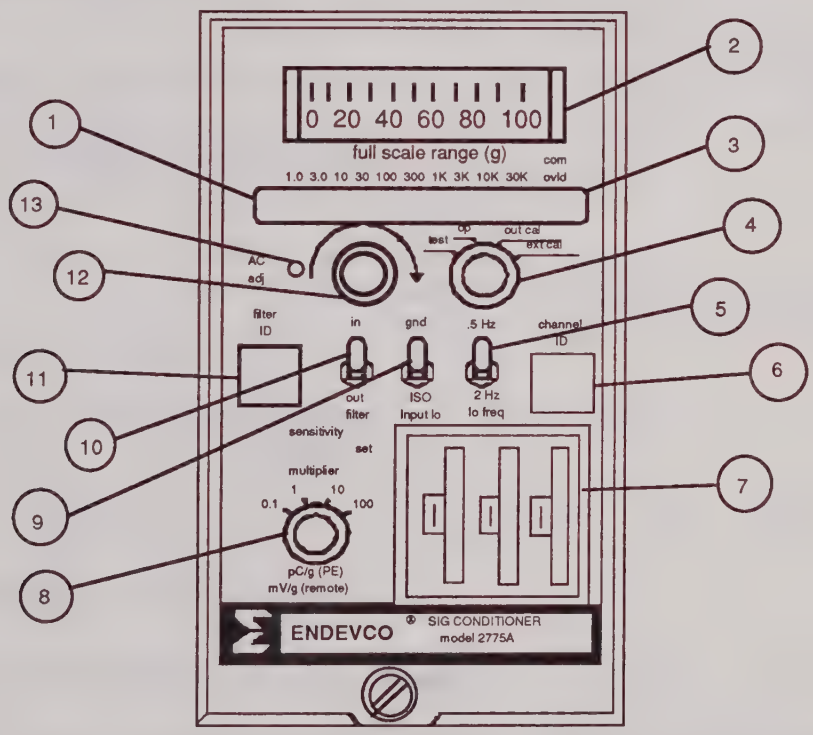

1	Full Scale Range (g) Indicator	8	Sensitivity multiplier switch
2	Percent of Full Scale Meter	9	Input Grounded - Isolated switch
3	Com Ovld Indicator Lamp	10	Filter in - out switch
4	Function switch	11	Filter ID Erasable Labeling Pad
5	0.5 Hz - 2 Hz Low Freq switch	12	Full Scale Range switch
6	Channel ID Erasable Labeling Pad	13	AC ADJ Potentiometer
7	Sensitivity Set Thumbwheel switch		

FIGURE 2-1: MODEL 2775A FRONT PANEL

A. SENSITIVITY SWITCHES

Two controls determine the amplifier input sensitivity, and they are a thumbwheel digital switch (Figure 2-1) and a multiplier switch that establishes a range of 0.1 to 1099 pC/g or mV/g sensitivity. Whether the controls represent pC/g or mV/g settings is dependent on the input mode selected; either a charge input from a PE transducer or a remote mV input from an Isotron transducer. The PE-RMT switch and the input connector on the rear panel must both correspond to the input mode of operation.

The sensitivity of the transducer in pC/g or in mV/g is entered as numerical digits into the thumbwheel switches (see Figure 2-2) and the multiplier switch is then placed to establish the decimal point. Be aware that not all of the ten available full scale settings shown on the Full Scale Range Indicator are permitted to be selected with any given sensitivity setting (table 2-1).

To establish the input sensitivity value for a given transducer or remote preamp device:

1. Enter the most significant digits of the transducer sensitivity (obtained from the transducer calibration certificate) into the thumbwheel switches. If the input is from a remote charge converter or integral electronics transducer, enter the transfer value.

2. Use the MULTIPLIER switch to establish the decimal point corresponding to the transducer sensitivity or the transfer value.

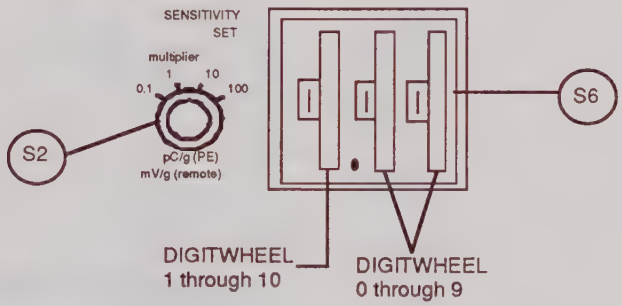

FIGURE 2-2: SENSITIVITY AND FULL SCALE SELECTION

Sensitivity Multiplier	Sensitivity Ranges	Selectable Full Scale Ranges
.1	.100 to 1.099	100,300, 1K, 3K, 10K, 30K
1	1.00 to 10.99	10, 30, 100, 300, 1K, 3K
10	10.0 to 109.9	1, 3, 10, 30, 100, 300
100	100 to 1099	1, 3, 10, 30

TABLE 2-1: SENSITIVITY AND FULL SCALE RANGE SELECTION

B. FULL SCALE RANGE (g) INDICATOR

The FULL SCALE RANGE (g) indicator has ten full scale ranges that it can indicate: 1, 3, 10, 30, 100, 300, 1K, 3K, 10K, or 30K. An LED lamp lights up to indicate the full scale range selected by the Full Scale Range switch.

NOTE: The full scale ranges which are permitted to be displayed depends directly on the input sensitivity selected on the SENSITIVITY SET and MULTIPLIER switches. When you rotate the Full Scale Range switch (clockwise or counterclockwise) you will see that not every corresponding LED lamp lights up for each full scale demarcation; only those that indicate permissible gain ranges allowed by the automatic gain scaling capability of the amplifier light up. (Refer to Table 2-1).

The full scale ranges are normally expressed in peak units. In some instances for convenience, the ranges may be expressed in rms units. NOTE: When using rms units, the rms level (0.707 x V pk) should not exceed the AC output V pk established by the AC ADJ potentiometer (see Figure 2-1.) (The adjustable range for the AC ADJ is 1 to 10 V pk.) Note that the transducer sensitivity expressed in pC/g does not influence the selection of rms or peak readout since the expressed value is a ratio:

$$\frac{\text{pC}}{\text{g}} = \frac{\text{pC pk}}{\text{g pk}} = \frac{\text{pC rms}}{\text{g rms}}$$

The calculated values for mV/g at AC OUTPUT with a 10 V pk Full Scale (F.S.) setting are shown in Table 2-2. However, for any setting of the AC ADJ potentiometer, the mV/g at the AC OUTPUT can be determined for any full scale as follows:

$$\text{Millivolts Per g} = \frac{\text{Full Scale Voltage (Set by AC ADJ in millivolts)}}{\text{Full Scale Range Selected}}$$

For example, assume AC ADJ is adjusted for 6 V full scale (6000 millivolts) and the Full Scale Range (g) Selector is set for 3 g F.S., this calculates to:

$$\text{Millivolts Per g} = \frac{6000\ \text{mV}}{3\ \text{g}} = 2000\ \text{mV/g}$$

F.S. Volts at AC out via AC ADJ	Full Scale g Ranges									
	1	3	10	30	100	300	1K	3K	10K	30K
10V	10V	3.33V	1.0V	333mV	100mV	33.3mV	10mV	3.3mV	1.0mV	0.33mV
5V	5V	1.66V	500mV	166mV	50mV	16.6mV	5mV	1.6mV	0.5mV	0.16mV
3V	3V	1.0V	300mV	100mV	30mV	10.0mV	3mV	.0mV	0.3mV	0.10mV
1V	1V	333mV	100mV	33mV	10mV	3.33mV	1mV	0.3mV	0.1mV	0.03mV

TABLE 2-2: CALCULATION OF mV/g VALUES

C. AC ADJ POTENTIOMETER

The AC ADJ potentiometer (Figure 2-1 and Table 2-2) is used to adjust the AC full scale output voltage within a 1.0V to 10 V range to meet user requirements. The voltage is set at

the factory for a 10 V pk full scale output unless otherwise specified by the user at the time of delivery.

D. PERCENT OF FULL SCALE METER

An analog meter on the front panel (Figure 2-1) displays the measurand as a percentage of full scale, 0% to 100%.

E. COMMON-MODE OVERLOAD INDICATOR

A COM OVLD (common-mode-voltage overload) indicating lamp (Figure 2-1) lights up whenever the input common grounded/isolated mode switch is in the ISO INPUT position (input left isolated, i.e. floating) and the voltage between input common and output common exceeds 6 V pk.

F. FUNCTION SWITCH

The TEST/OPERATE/OUTCAL/EXTCAL selector switch (Figure 2-1) selects the operating mode. The OP (operate) position is selected for normal on-line test operation.

NOTE: Two light emitting diodes (LED's), separated by the 1 K indicating LED of the FULL SCALE RANGE display, will light up whenever the mode selector switch is placed at a position other than at OPERATE.

When the TEST position is selected, an external signal may be injected through the rear panel TEST connector to the piezoelectric transducer input shielding. This permits testing of the transducer to signal conditioner connection.

When the OUT CAL (output calibration) position is selected, an internal full scale signal is applied to the AC and DC output stages in order to generate a output voltage for calibration of connected measuring or recording instruments. The SERVO output is not affected by the OUT CAL mode.

When the EXT CAL (external calibration) position is selected, the EXT CAL input is connected to the charge converter input through an internal 1000 pf +0.5% capacitor to convert the mV input to pC charge input.

NOTE: When EXT CAL is not in use, the BNC connector should have a shorting cap or remain connected to a low impedance source to reduce possible pick-up of noise.

G. INPUT GROUNDED/INPUT ISOLATED SWITCH

The INPUT GROUNDED/INPUT ISOLATED switch (Figure 2-1) ties the input ground to the output ground when in the GND position. When placed in the ISO position, the input ground is isolated from output common. This may be used to prevent ground loops in the system by floating the accelerometer input ground.

H. 0.5 HZ LOW FREQ/2 HZ LOW FREQ SWITCH

When the 0.5 HZ LOW FREQ/2 HZ LOW FREQ switch (Figure 2-1) is placed at 0.5 Hz, the gain is -5% of midband gain at 0.5 Hz (-3 dB at 0.2 Hz). When the switch is placed at 2 Hz, the gain is -5% of its midband gain at 2 Hz (-3 dB at 0.6 Hz).

NOTE: On some units the 0.5 Hz is marked >.1 Hz which indicates the -3db point instead of the -5% point.

I. FILTER IN/FILTER OUT SWITCH

The FILTER IN/FILTER OUT switch (Figure 2-1), when placed at FILTER IN, allows processing of the incoming signal through an optional Model 35771 internally installed filter. The unit is shipped from the factory with a jumper connector in place so the filter switch will not affect the data unless the jumper is removed or the filter is installed. See section six for Model 35771 filter option specs.

J. CHANNEL/FILTER ID PADS

Two labeling pads FILTER ID and CHANNEL ID (Figure 2-1) on the front panel permit the user to pencil in the type of filter, if installed, and the channel ID number.

3. REAR PANEL CONTROLS

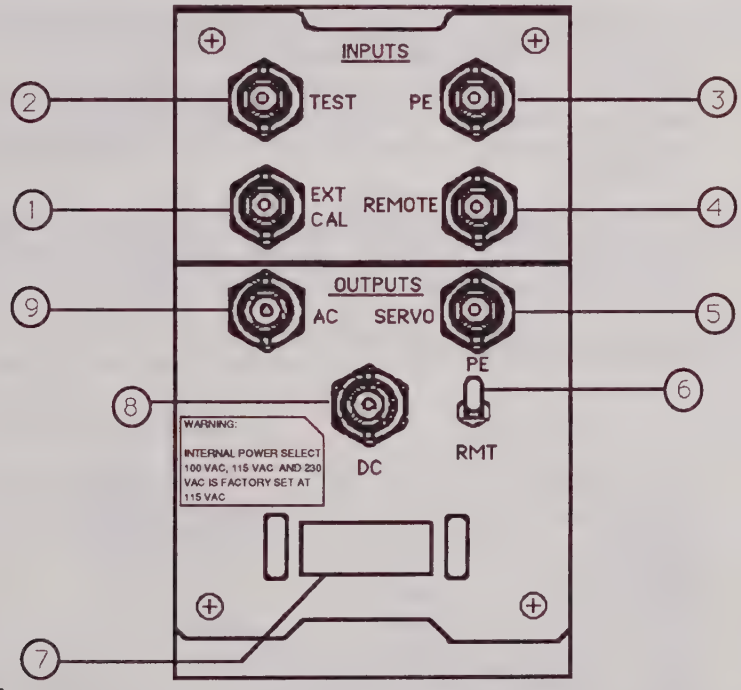

1	EXT CAL INPUT Connector	6	PE-REMOTE Switch
2	TEST INPUT Connector	7	AC INPUT POWER Connector
3	PE INPUT Connector	8	DC OUTPUT Connector
4	REMOTE INPUT Connector	9	AC OUTPUT Connector
5	SERVO OUTPUT Connector		

FIGURE 2-3: REAR PANEL CONTROLS AND CONNECTORS

A. INPUT/OUTPUT CONNECTORS (See Figure 2-3)

The PE input receptacle is a miniature coaxial 10-32 thread type. All other input and output receptacles REMOTE, TEST, EXT CAL, AC, DC and Servo are BNC Type UG-1094/U or equivalent. A Microdot, 10-32 to BNC Adapter (P/N EJ21) is used to adapt a BNC connector to the miniature coaxial 10-32 plug used on low noise cable assemblies.

B. PE/REMOTE SWITCH

The PE/REMOTE Switch determines the mode of operation for the signal conditioner: PE for direct connection to a piezoelectric transducer and RMT for connection to an Isotron transducer or remote charge converter. The corresponding PE input or REMOTE input connector must be used for proper operation.

C. POWER CONNECTIONS (See Figure 2-3)

The power connector is a 3-prong Cinch\ P-303. The third wire of the power connector is connected to chassis ground.

NOTE: GND No. 1 (input ground) and GND No. 2 (output ground) are delivered from the factory insulated from chassis ground. However, the customer has an option to connect GND No. 2 (output ground) to chassis ground by soldering a jumper across circuit pads E4 and E5 on the signal conditioner circuit board (See Figure 2-4). Output ground and chassis ground are normally connected through external test equipment or recording devices third wire ground.

When the signal conditioner is installed in the Model 4948 Adapter, the power connector mates with a receptacle on the inside rear of the Model 4948. The adapter frame and the signal conditioner chassis are grounded by the third wire from the power source.

4. INTERNAL CONTROLS

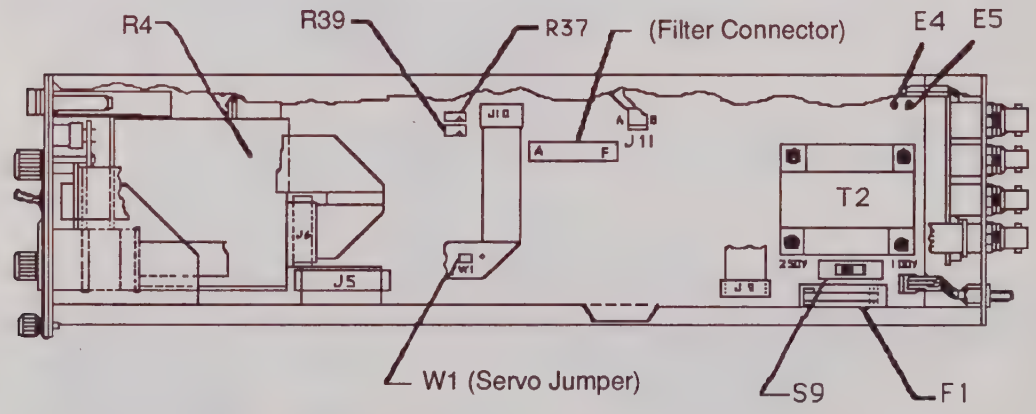

FIGURE 2-4: INTERNAL CONTROLS

A. POWER LINE INPUT SELECTOR

The Power Line Input Selector switch (Figure 2-4) configures the Model 2775A to operate from 50 to 400 Hz power at one of the following voltage ranges:

Switch Position		VOLTAGE RANGE
POS 1	100 V	90 - 110 V rms
POS 2	115 V	105 - 125 V rms
POS 3	230 V	210 - 250 V rms

B. FUSE

A fuse, Fusetron, 1/4 A, Type MDL 250-volt, Slo-Blo, or equivalent, is connected in series with the power line. The same fuse is used for all power ranges (See Figure 2-4).

C. SERVO OUTPUT VOLTAGE RANGE SELECTION

Jumper clip W1 is used to select the fixed mV/g ratio for the servo output. It can be set for either 10 mV/g or 100 mV/g by jumping the appropriate two pins, see Figure 2-4.

NOTE: The factory setting is 10 mV/g.

D. FILTER CONNECTOR

Connector J15 (Figure 2-4) permits installation of an optionally provided Model 35771 plug-in filter assembly (high-pass, low-pass, or bandpass.) The filter assembly is held in place by a captive screw. (Refer to Section 6 for the Model 35771 specifications.)

The FILTER IN/FILTER OUT front panel switch provides for user control of the filter. Connector pins are identified as follows:

PIN	-	FUNCTION
A	-	Signal Input
B	-	Signal Output
C	-	Signal and Power Ground
D	-	-15 Vdc
E	-	+15 Vdc
F	-	No Connection

E. ADJUSTMENT POTS

The constant current adjust pot, R4, adjusts the constant current level at the REMOTE input connecter. The adjustment range is <0.5mA to >20mA. Refer to section 5.15 for the adjustment procedure.

The common mode adjust pots, R37 and R39, are adjusted to achieve minimum common mode voltage at the AC output when operating in the floating (isolated) ground mode. Refer to section 5.4 for the adjustment procedure.

SECTION 3
OPERATING INSTRUCTIONS

1. UNPACKING AND INSPECTION

The equipment has been thoroughly inspected and tested at the factory, and should be ready for operation when received. The customer, however, should make an inspection to be certain that no damage has occurred during shipment.

Carefully remove the instrument from its packing box. Inspect each item shipped for any sign of damage. Obvious damage should be reported immediately to the carrier.

Inspect each shipping carton and verify that the contents conform to the items of equipment listed on the Packing List. Notify the factory if a discrepancy exists between the Packing List and the contents received.

2. INSTALLATION

The Model 2775A signal conditioner is completely self-contained and may be operated on a bench, or in the Model 4948 Rack Adapter. Up to six units may be mounted in the Model 4948 Rack Adapter and are held in place by a knurled screw located at the bottom of each front panel.

Proper ventilation is required around the instrument when installed in the Model 4948 rack adapter. The top and bottom of the 4948 adapters are open to allow circulation of air. To maintain specification limits and tolerances the air temperature around the 2775A signal conditioners should not be allowed to go higher than +125°F (+52°C) when the instruments are in operation. Rack separation of several inches and or cooling by forced air or convection may be required.

CAUTION: Before applying power make sure the 2775A is correctly set to operate from the local power source to prevent damage to the equipment. DO NOT switch the LINE POWER selector with power applied.

The line power selector is factory set to 110V, if the power available is different, set the LINE POWER selector switch inside the Model 2775A to the correct power line setting (see Figure 3-1).

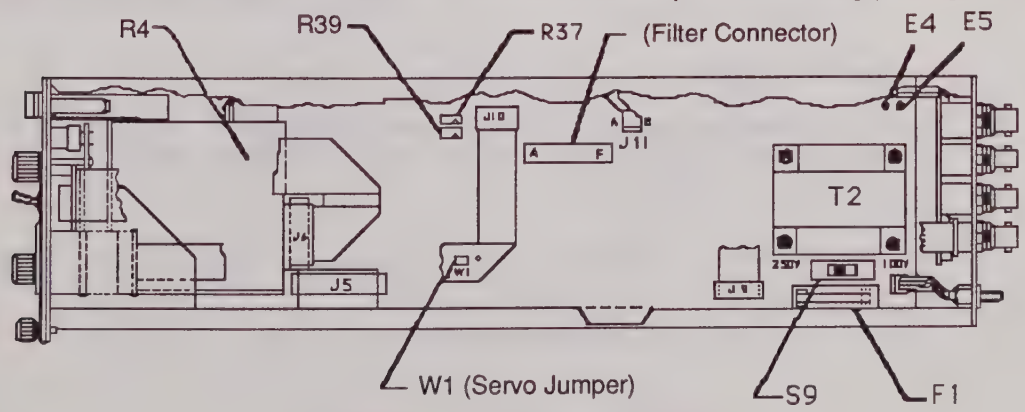

FIGURE 3-1: INTERNAL CONTROLS

Line Power Selector	Power Source
POS 1 100 V	90 to 110 Vac, 50 to 400 Hz
POS 2 100 V	105 to 125 Vac, 50 to 400 Hz
POS 3 230 V	210 to 250 Vac, 50 to 400 Hz

The three-wire power cord for 100- or 115-volt power line operation is terminated in a standard three-prong plug. (For 230-volt operation the plug is not supplied and the ends of the wires are stripped and tinned for installation of an outlet plug from a local supplier.

GROUNDING

The chassis is connected to the third wire ground of the power plug. Insulated guide rails in the Model 4948 rack adapter ensure electrical separation of the amplifier signal grounds from other amplifiers. To prevent pickup of stray electrical noise, it may be required to connect the signal output ground (Gnd No. 2) to third wire ground via external equipment or chassis ground. This also may be done by soldering a jumper between E4 and E5 pads on the circuit board (see figure 3-1).

NOTE: Multiple ground points in any one data channel must be avoided to prevent ground loops.

3. CHECKOUT

A. EQUIPMENT REQUIRED

The following equipment is required for checkout:

DVM	True RMS Voltmeter 0.1% accuracy or better (fluke 8050A or equivalent)
Oscilloscope	General Purpose Oscilloscope 10 MHz bandwidth or greater (Tektronix 2213A or equivalent)
Signal Generator	Synthesizer/Function Generator 0.1Hz to 100 KHz (Hewlett Packard 3310A or equivalent)
Frequency Counter	Multi-Counter (fluke 1900A or equivalent)

B. INITIAL SETUP

On the back panel, set the MODE switch (S5) to PE. On the front panel, from top to bottom, left to right, set the following controls as indicated (figure 3-2).

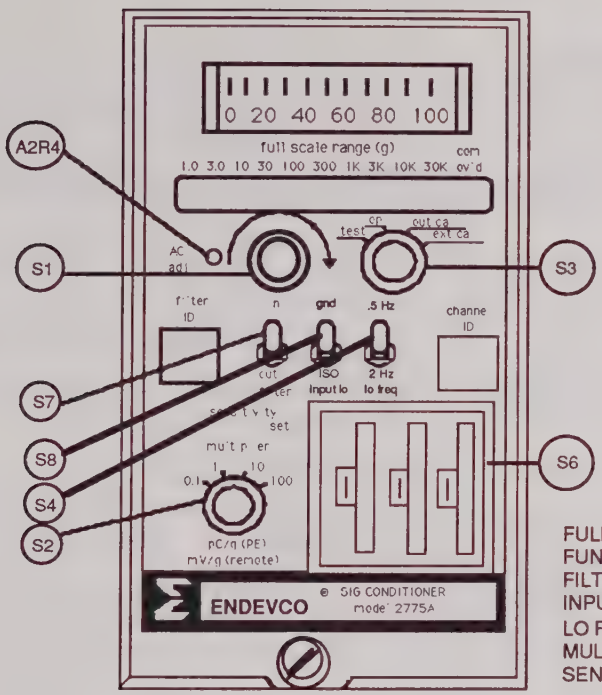

FULL SCALE control (S1) to 10
FUNCTION switch (S3) to OUT CAL
FILTER switch (S7) to OUT
INPUT LO switch (S8) to GND
LO FREQ switch (S4) to 2 Hz
MULTIPLIER switch (S2) to 1
SENSITIVITY switches (S6) to 1.00

FIGURE 3-2: FRONT PANEL CONTROLS

C. OUTPUT CAL

Set the FUNCTION switch (S3) to OUT CAL. Monitor AC OUTPUT (J12) with a Frequency Counter and an oscilloscope and verify that the internal oscillator sine wave is between 950 and 1050 Hz (Figure 3-2).

Monitor the AC OUTPUT (J12) with a DVM in the rms mode for a full scale ±1% reading. This output should be between 7.00 and 7.14 V rms (10 V pk) which is the factory calibrated setting or should be the user specified full scale level needed for operational use. Refer to section 5 for AC output adjustment.

Monitor DC OUTPUT (J14) with a DVM for a 10 Vdc ± 150 mV full scale reading.

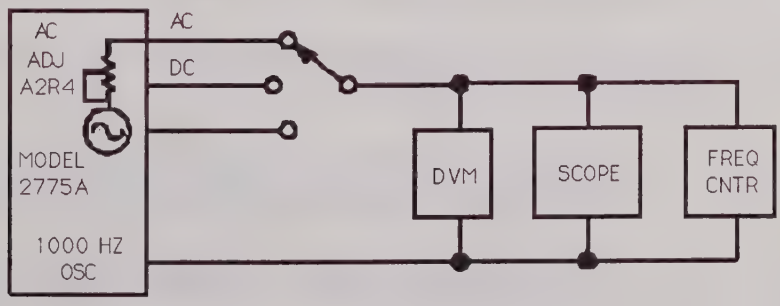

FIGURE 3-3: OUTPUT CALIBRATION DIAGRAM

D. EXTERNAL CAL INPUT

Set the FUNCTION switch (S3) to EXT CAL and apply 10mV pk (7.07mV rms) at 1 kHz into EXT CAL INPUT and measure the AC OUTPUT (J12) for a full scale ±3.0% reading. This output should be between 6.86 and 7.28 V rms which is the factory calibrated setting or should be the user specified full scale level needed for operational use.

Set S1 at 100 and the input voltage at 100 mV pk (70.7 mV rms). Measure servo output for 1 V pk (.707 V rms) ± 2.0%.

NOTE: When external cal is not in use, leave connected to a low impedence source or install a shorting cap to prevent noise pick-up.

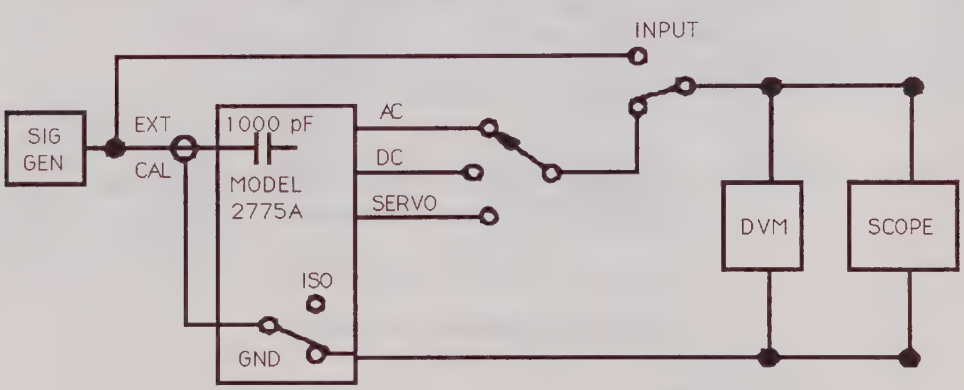

FIGURE 3-4: EXTERNAL CALIBRATION INPUT

4. OPERATION

Before utilizing the signal conditioners, the operator should be thoroughly familiar with the controls and with signal levels available at the output connectors. A complete knowledge of the instrument will ensure that meaningful data is obtained. It is recommend that all of this manual, particularly Sections one, two and the specifications in the data sheet (at the back of this manual) be understood before attempting to make a measurement.

A. MONITORING ACCELERATION OR OTHER MEASURANDS

To prepare the Model 2775A for conditioning the signal from a transducer, the following procedure is recommended:

1. Establish a desired full scale AC output voltage. This voltage is adjustable from 1 to 10 V pk by means of the AC ADJ potentiometer (See Figure 3-2.) It is normally set at the factory for a full scale output of 10 volts peak unless specified otherwise.

   To change the full scale AC output voltage, set the FUNCTION switch to OUT CAL, and adjust AC ADJ potentiometer for the desired full scale output. (Refer to calibration procedure in Section 5).

2. From the calibration record card supplied with the transducer, note the charge sensitivity expressed in pico coulombs per g (pC/g).

3. Adjust the SENSITIVITY SET switches to indicate the transducer sensitivity and set the sensitivity MULTIPLIER to establish the decimal point for the sensitivity determined in Step 2. (Refer to paragraph 2.1).

4. Set the front panel switches to the following positions:

   a) Function switch to OP (operate)
   b) Input isolation switch to GND
   c) LO FREQ to 2 HZ or 0.5 Hz (some units marked >.1 Hz)
   d) Filter switch to IN or OUT

5. Connect the input device to the appropriate input on the rear panel: PE INPUT or REMOTE INPUT AND PLACE THE INPUT MODE switch in corresponding position.

   NOTE: It is recommended to keep the amplifier in the grounded position during hookup. Always turn off the amplifier before connecting an Isotron accelerometer to prevent damage to the internal electronics.

   To minimize the effect of unavoidable ground loops, the signal conditioner can be operated in the Isolated Mode. In this mode the input common ground is insulated from output common ground; i.e., the input is left floating.

6. Apply power to the signal conditioner and turn the Full Scale Range control until the desired full scale range is indicated by the LED indicator (See Table 2-1 for the available full scale ranges.) The signal conditioner will be ready for use in less than five minutes; however, it may not meet all specification requirements until it has warmed up for 30 minutes.

7. Whenever a full-scale output signal for setup calibration of recording instruments is needed, place the operating mode selector switch at the OUT CAL position. The AC and DC output signals will represent peak full scale outputs regardless of the input sensitivity and full scale range settings.

   NOTE: When the operating mode selector switch is in OUT CAL, the input signal to the signal conditioner is disconnected.

8. Return the operating mode selector switch to the OP position.

9. The Servo output may be selected for 10 mV/g or 100 mV/g by a jumper clip on the main circuit board. The Servo output is independent of the full scale g range selected. The top cover must be removed to set the servo jumper clip (see Figure 3-1).

   NOTE: The top cover is grounded to the chassis by the screws at the top of the signal conditioner. These screws must be tightened in place at all times to ensure proper shielding of the components within the signal conditioner.

   NOTE: When the Servo output is used for shaker control, DO NOT CHANGE FULL SCALE RANGES WHILE THE SHAKER IS IN OPERATION. Switching transients may appear on the Servo line causing a change in shaker response resulting in over or under test of articles on the shaker.

10. The signal conditioner is now ready to accept the signal from the transducer. The number of engineering units (g, lbs, psi, etc.) represented by the output voltage is equal to the voltage divided by the system sensitivity, expressed as follows:

$$\text{Engineering Units} = \frac{\text{AC Peak Volts Out}}{\text{System Sensitivity}} \quad (1)$$

Where:

$$\text{System Sensitivity} = \frac{\text{Full Scale Output [V pk]}}{\text{Full Scale Range [g pk, lb}_f\text{, pk, etc.]}} \quad (2)$$

$$\frac{\text{volts pk}}{\text{g pk}} = \frac{\text{volts rms}}{\text{g rms}} = \frac{\text{volts}}{\text{g}}$$

To solve a typical example of the engineering units represented by the AC output voltage, assume:

a) The Full Scale AC Output is adjusted to 10 V pk (AC ADJ pot.)

b) The Full Scale Range is set for 1000 g pk.

c) An 8 V pk signal is present at the AC OUTPUT. Determine the g level represented by the 8 V pk at the AC OUTPUT.

First, using formula (2), calculate for system sensitivity

$$\text{System Sensitivity} = \frac{\text{10 V pk}}{\text{1000 g pk}} = 0.010 \text{ V/g}$$

Then using the calculated system sensitivity value, the AC OUTPUT reading of 8 V pk, and formula (1),

$$g = \frac{\text{8 V pk}}{\text{0.010 V/g pk}} = 800 \text{ g}$$

To express accelerometer sensitivity in pC/m/s^2, divide sensitivity in pC/g by 9.807. (Precise conversion is 1 g = 9.80665 m/s^2.)

B. AC OUTPUT

The full scale AC output voltage will depend on the setting of the AC ADJ potentiometer (Figure 3-2), and is adjustable from 1 to 10 volts peak. It is normally set at the factory for 10 volts peak except when specified otherwise. The AC output is capable of delivering up to 85 mA pk, which is sufficient to drive most high frequency galvanometers or long cables.

Both input and full scale output should be expressed in peak units. The input measurand may be expressed in rms units by converting from peak units; however, assure that the maximum peak specified is not exceeded by converted rms levels.

The signal at the AC output connector is in phase with the input signal when the internal filter is not used or when the 35771 selectable Filter is installed. However, when low pass or high pass active filters (such as 35257 OR 35330 series) are selected, the output signal is inverted with respect to the input. The model 2771A-X remote charge converter inverts the input signal 180 degrees.

C. OUTPUT CALIBRATION

Placing of the operating mode selector switch at OUT CAL disconnects the signal conditioner input and connects an internal sinusoidal oscillator to one of the intermediate output stages. The signal is processed and its amplitude represents the full scale peak of the measurand regardless of the position of the input sensitivity switches and Full Scale Range selector switch. Recording instruments connected to the AC and DC outputs can be calibrated for peak full scale.

D. EXTERNAL CALIBRATION

When you need to check the operating condition of the Model 2775A, the EXTERNAL CAL input can be used. Calculate the oscillator V pk signal value needed for a desired peak AC full scale output. The AC OUTPUT will be 10 V pk if the factory adjusted voltage is unchanged or will be whatever user selected voltage has been set by the AC ADJ pot. To obtain full scale output, the voltage input in mV should be:

V_{in} [mV] = F.S. x S

Where: F.S. is the full scale and S is the sensitivity setting
(This is the input voltage for peak full scale output.)

Verify that the amplifier output is within 2.0% of full scale for the expected AC, DC or Servo Output.

E. TEST INPUT

An external sine wave oscillator can be connected to the TEST INPUT connector to insert a signal in series between the transducer and input of the charge amplifier. The signal is transformer coupled and is applied to the PE cable shielding when the mode select or switch is in the TEST position (See Figure 4-3 in Section 4). The test input can be any voltage which will give a convenient reading at the output. The test frequency must be between 100 and 10 000 Hz. If the transducer signal return is grounded to the test structure, the amplifier must be operated in the Floating (isolated) mode. Figure 3-5 shows the Input Grounded mode.

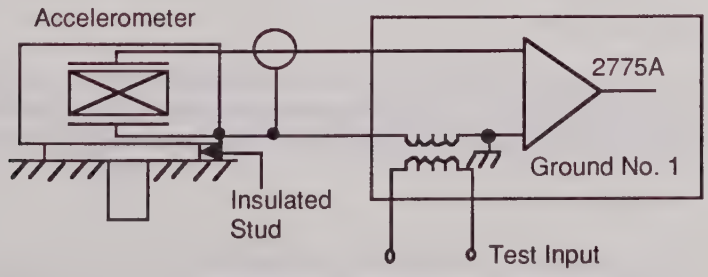

FIGURE 3-5: TEST INPUT

This test signal is normally used to verify tat the transducer and its cable are properly connected. A predictable output is produced when the test signal amplitude is adjusted to the value calculated as follows:

$$E_t = \frac{GS}{C_p + C_c} = \text{volts peak}$$

Where:
- G = peak amplitude of simulated signal; g, psi, lbs, etc.
- S = charge sensitivity of transducer, pC/g, pC/psi, etc.
- C_p = capacitance of transducer, pF
- C_c = capacitance of input cable, pF

If G is equal to the setting of the Full Scale Range switch, the output voltage will be at approximately calibrated full scale.

If the cable and signal conditioner are connected properly, the charge "seen" by the charge amplifier will be:

$$Q = Et\ (Cp + Cc)\ pC\ pk$$

If the transducer is disconnected, the input charge will be:
Q1 = Et (Cc) and the output voltage will be reduced from the anticipated magnitude by a factor of Cc/(Cp + Cc)

Because the Test Input signal is transformer coupled, any number of Test Input terminals may be connected to one signal generator with a common ground. The Test Input feature cannot be used in the remote mode of operation. It can be used when the input ground is isolated from output common.

F. SERVO OUTPUT

The Model 2775A provides a servo signal voltage proportional to the input signal scaled for either 10 mV/g or 100 mV/g. (The mV/g setting is internally selected by a moveable jumper clip. It is set at the factory at 10 mV/g.)

The output is an unfiltered (broadband) signal in phase with the input signal. Specified maximum signal linearity is 12 Vpk. Assuming that the servo output is set for 10 mV/g, the maximum g level for an undistorted servo signal is 1200 g regardless of sensitivity or full scale settings. (For a 100 mV/g servo output setting, the maximum is 120 g).

G. DC OUTPUT

The Model 2775A provides a DC voltage at the DC output connector proportional to the average value scaled to pk of the input signal. With a sinusoidal full scale input signal, the full scale DC output is +10 volts peak. Maximum output current is 3.0 mA.

H. PANEL METER

The meter obtains its signal from the AC-DC converter and, therefore, responds to the average magnitude of the input signal scaled to pk. It indicates percentage of full scale and is most accurate for sinusoidal input signals.

I. FILTER

The FILTER IN/FILTER OUT front panel switch permits for user control of the internal filter. An optionally provided Model 35771 selectable filter card is adjustable to function as a low-pass, high-pass or bandpass filter. Refer to Section 6 for the available cut-off frequencies or for the calculation of customized cut-off frequencies.

Two earlier model series of filters (which may exist in your inventory) can be used in the 2775A Signal Conditioner; however, the inversion factor of the active high and low-pass filters must be taken into consideration. The Model 35257 is a series of low pass filters; the Model 35330 is a series of high pass filters. Both of these series are active two-pole Butterworth designs providing 12 dB per octave roll-off. The AC output signal is inverted with respect to the input when these filters are selected.

J. FLOATING INPUT OPERATION

If the transducer signal return wire is connected (grounded) to the test structure, it may be desirable to isolate the input ground from output ground to prevent a ground loop or stray pick-up. When the INPUT LO GND/ISO switch is in the INPUT ISO (floating) position, input and output (common grounds are insulated from each other by 50 megohms minimum. The Model 2775A will meet all specification requirements with up to 6 volts peak common-mode-voltage. No damage will occur to the circuits with a common-mode-voltage up to 500 volts peak.

The Common Mode (COM OVLD) Overload LED lamp will light when the common-mode-voltage input exceeds 6.5V ±7%. When this occurs, steps should be taken to reduce the common-mode-voltage. It may be necessary to insulate the transducer from ground with an insulated stud. If the transducer is insulated from the test structure, the signal conditioner should be operated in the Grounded mode.

The Test Input feature may be used with the signal conditioner operated with the input in the Grounded or Floating mode.

K. USING LONG INPUT CABLES

The maximum allowable source capacitance, to meet all specifications, is 30 000 pF. Source capacitance includes both transducer and input cable capacitance. An input capacitance greater than that specified above will result in increased residual noise and reduced frequency response from the amplifier.

L. REMOTE PREAMP

An Isotron transducer or remote charge converter (or remote preamp) may be connected to the Model 2775A with standard coaxial or low impedance, shielded, twisted-pair cable. The cable carries the DC power to the remote preamp device and, at the same time, carries data signals to the Model 2775A.

When the PE-RMT INPUT MODE switch is at the remote (RMT) position, the internal Charge Converter circuit is disconnected and replaced with the Preamp Input Conditioner circuit. All features of the Model 2775A Signal Conditioner, except Test Input, and External Cal may be used when operating in the remote mode. No damage will occur if the switch is in the remote (RMT) position without a remote preamp connected to the input.

M. REMOTE INPUT INTERFACE FACTORS

There are four principal factors to be aware of when connecting the remote input. These factors are: (1) the constant current specified for the remote device (preamp) to be connected, (2) the compliance voltage of the constant current source, (3) the specified bias voltage at which the remote device operates, and (4) the high frequency response limitations of the remote device to 2775A coupling system.

CAUTION: Turn the 2775A off before connecting Isotron accelerometers to the remote input. This prevents damage to the internal electronics of the transducer due to capacitance discharge of the cable.

Knowledge of the constant current rating for the remote device is important so as not to exceed its constant current handling capabilities when connected to a current source. (NOTE: The 2775A has an adjustable 0..5 to >20 mA constant current source. Refer to Section 5 for the Constant Current Adjustment procedure. Do not leave adjusted higher than 20 mA to prevent damage to Isotron accelerometers.)

The compliance voltage level and the remote device bias voltage are factors that determine the signal transfer characteristics of the device. Figure 3-6 shows the transfer characteristics of the device Figure 3-6 shows the transfer characteristics of a typical remote preamplifier. In the 2775A, the compliance voltage is 21 Vdc, the AC maximum is 20 V pk-pk, and the combined AC and DC components cannot exceed 25 volts.

To illustrate signal transfer, assume we have a representative Isotron accelerometer which operates at a bias level of 10.0V nominal and can handle up to 20 mA of constant current. (See Figure 3-6) Refering to Figure 3-7, one can see that the 10.0V operating bias level and the 2775A compliance voltage of 21 Vdc allows a 20 V pk-pk AC signal to be transferred without clipping.

High frequency response limitations must also be considered when using long cable to couple a remote device to the 2775A. The current that is available to drive a coaxial cable, the peak signal level, and the cable capacitance are all important and interrelated factors that determine frequency response of the coupling system.

Again, let us use our representative Isotron transducer as an example to illustrate frequency response. Assume that the 2775A is adjusted to provide 10 mA of constant current. Of the 10 mA, assume 1 mA is needed for device operation without distortion; therefore, up to 9 mA are available to drive the capacitance load inherent in a cable.

Referring to Figure 3-8, the nomograph shows the frequency response for a given cable capacitance as a function of peak AC voltage and the available drive current. The relationship of volts peak to available current is: v/mA. Take the 10 pk that the 2775A can handle, dividing this by the 9 mA available drive current gives us 1.1V per mA. Using the nomograph, Figure 3-8, one can determine the approximate maximum frequency that can be transmitted for any given cable capacitance. (i.e., 14 kHz for 10,000 pF cable capacitance.)

For instance, assume that your coaxial cable in this case is 100 feet long. Thus, you have 3,200 pF of capacitance (coaxial cable capacitance is 32 pF/ft typical.) From the nomograph, this capacitance and the 1.1 volt per mA value yields a maximum frequency response of approximately 49 k Hz. This cable length, therefore, is satisfactory for the 2775A REMOTE input. The frequency response with a remote input is dependent on the Full Scale and Sensitivity multiplier settings and can be a s high as 70 kHz. (See specifications.)

An alternative to using the nomograph is to calculate the frequency response. Generally, the highest frequency that can be transmitted without current limiting is:

$$f_{max} = \frac{I}{2 \pi V C} \quad (1)$$

Where I is maximum available drive current in amperes, V is peak sine wave signal in volts, and C is capacitance in picofarads.

A coupling system with longer cable lengths can be used for single transfer, but only if AC sine wave signals of low amplitude are transmitted. This is because a larger capacitive load (longer cable) can be driven by lower amplitude signals. This relationship can be seen from equation (1).

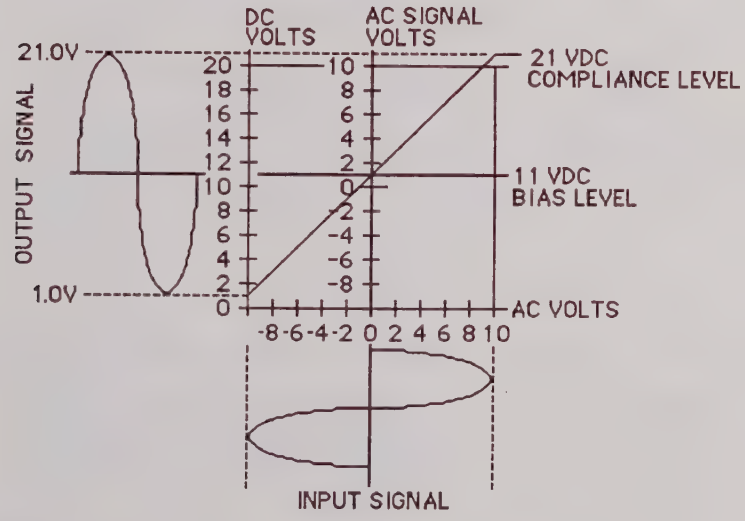

FIGURE 3-6: REMOTE TRANSFER

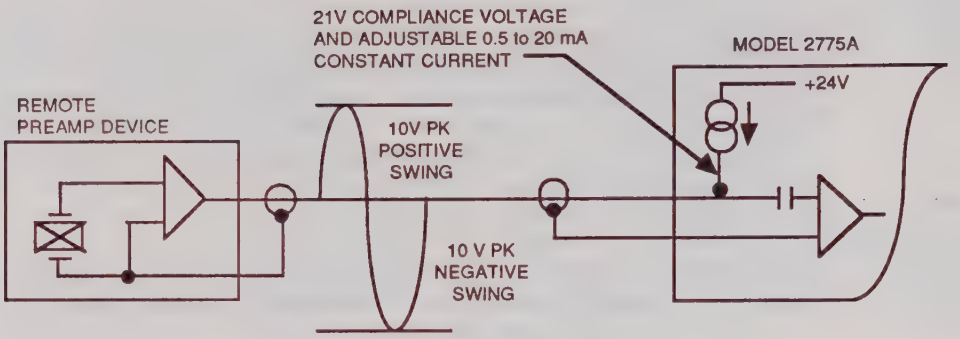

FIGURE 3-7: REMOTE HOOKUP

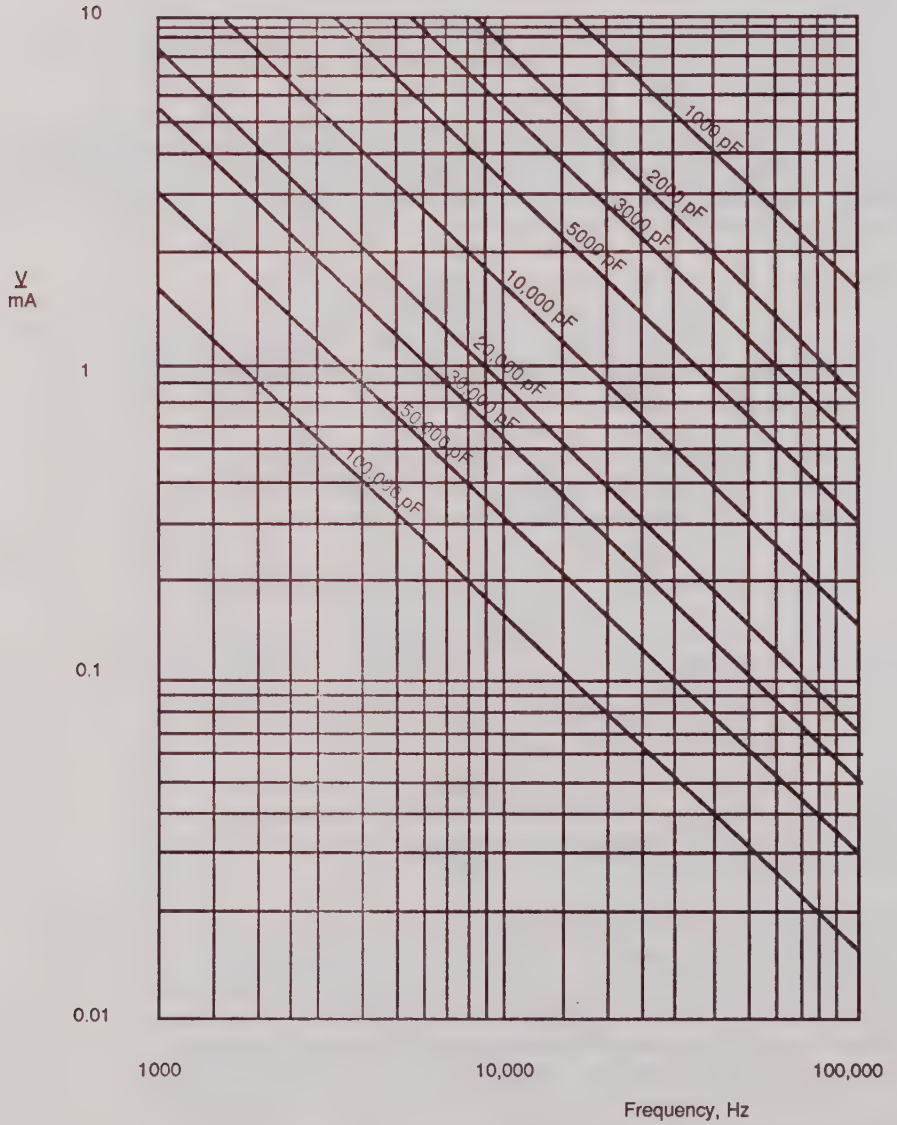

FIGURE 3-8: FREQUENCY RESPONSE NOMOGRAPH

SECTION 4
THEORY OF OPERATION, CIRCUIT DESCRIPTION AND SPECIFICATIONS

1. THEORY OF OPERATION

A. CHARGE GENERATORS

Piezoelectric transducers are self-generating devices and require no electrical excitation. The electrical charge that is generated is proportional to the stress on the piezoelectric crystal. In an accelerometer, the output is proportional to acceleration; in a pressure transducer, the output is proportional to pressure, etc. For any transducer, the charge generated is independent of the amount of external capacitance attached to the transducer.

The simplified equivalent circuit of a piezoelectric or capacitive transducer is shown in Figure 4-1. The open circuit voltage is equal to the charge (q) divided by the transducer capacitance (C_p),

$e_o = q/C_p$ where e_o is expressed in volts, q in pico coulombs, and C_p in picofarads. If the open circuit voltage is known, the charge can be calculated from $q = e_o Cp$.

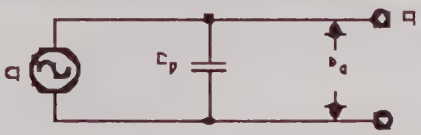

FIGURE 4-1: SIMPLIFIED EQUIVALENT CIRCUIT

All Endevco PE transducers are provided with a calibration certificate which specifies the charge sensitivity expressed in pico coulombs per unit measurand. For an accelerometer, the sensitivity is given in pC/g where:

$$Q_s = \frac{pC}{g} = \frac{pC\ pk}{g\ pk} = \frac{pC\ rms}{g\ rms}$$

For transducer sensitivities given only in terms of voltage, the charge sensitivity can be calculated from:

$$Q_s = \frac{E_{cal}\,(Cp + C_{cal})}{1000}$$

Where:

Q_s	=	charge sensitivity, in pC/g
E_{cal}	=	factory supplied voltage sensitivity, in mV/g
Cp	=	internal capacitance of transducer, in pF
C_{cal}	=	external cable and amplifier capacitance, in pF

The values of E_{cal}, C_p, and C_{cal} are usually given on the calibration certificate. Since the charge sensitivity is not affected by capacitance connected external to the transducer, no additional calculations are necessary.

For example, the nominal voltage sensitivity (E_{cal}) of the Endevco Model 2272 Accelerometer is 4.0 mV/g, nominal capacitance is 2700 pF, and the accelerometer is calibrated with 300 pF of external capacitance. Thus, the nominal charge sensitivity is:

$$Q_s = \frac{4\,(2700 + 300)}{1000} = 12 \text{ pC/g}$$

B. CHARGE CONVERSION

The input circuit of the Model 2775A consists of a charge converter which accepts the electrical charge from the transducer and converts it to a voltage proportional to the input charge. The charge converter is essentially a voltage amplifier with capacitance feedback, Figure 4-2. In operation, the output voltage which occurs as a result of the charge input signal is fed back through the feed-back capacitor C_f in such a direction as to maintain the voltage at the input at, or very close to, zero. Thus, the input charge is stored in the feedback capacitor, producing a voltage across it which is equal to the input charge divided by the capacitance of the feedback capacitor.

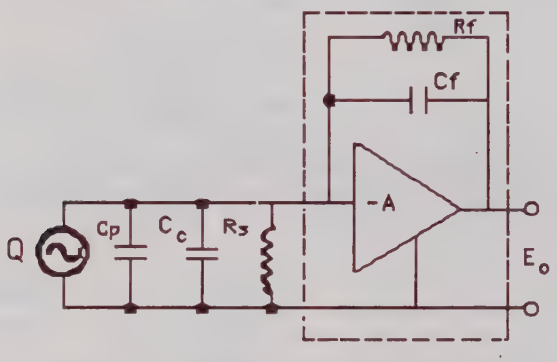

FIGURE 4-2: CHARGE CONVERTER CIRCUIT

The transfer characteristic (conversion gain in mV/pC) of the charge converter depends primarily on the value of the feedback capacitor. When the amplifier is operated within specification limits, the equation for conversion gain simplifies to the relationship:

$$\frac{E_o}{Q} = \frac{1}{C_f}$$

In effect, a charge converter is a circuit which appears to have a capacitance input impedance so large that the effect of varying input transducer or cable capacitance is insignificant. Thus, large variation of source capacitance is possible without any appreciable change in overall system sensitivity.

C. LOW FREQUENCY RESPONSE

In many applications, particularly when using transducers with ceramic crystals, it is desirable to eliminate quasi DC outputs which can be produced in the transducer due to pyroelectric effects. For most shock and vibration measurements, flat frequency response is required only at frequencies down to about 2 Hz. Thus, the addition of a feedback resistor R_f in parallel with the feedback capacitor results in control of the low frequency response of the circuit and a low frequency cutoff of:

$$f_c = \frac{1}{2 R_f C_f}$$

One of the advantages of the charge amplifier is that a desired low frequency response can be achieved in the amplifier design.

2. CIRCUIT DESCRIPTION

NOTE: See Figure 4-3 and refer to Schematic SC2775A in Section 7.

The Model 2775A Signal Conditioner can be regarded as comprising:
(1) an input stage (charge converter or preamp input conditioner), (2) an isolation amplifier (for common mode rejection when needed), (3) a sensitivity normalization stage, (4) a gain stage, (5) gain control logic, and (6) AC, DC, and Servo output stages. A 1 kHz internal oscillator is included to generate a CAL OUT signal, and a power supply furnishes all necessary power for circuit operation.

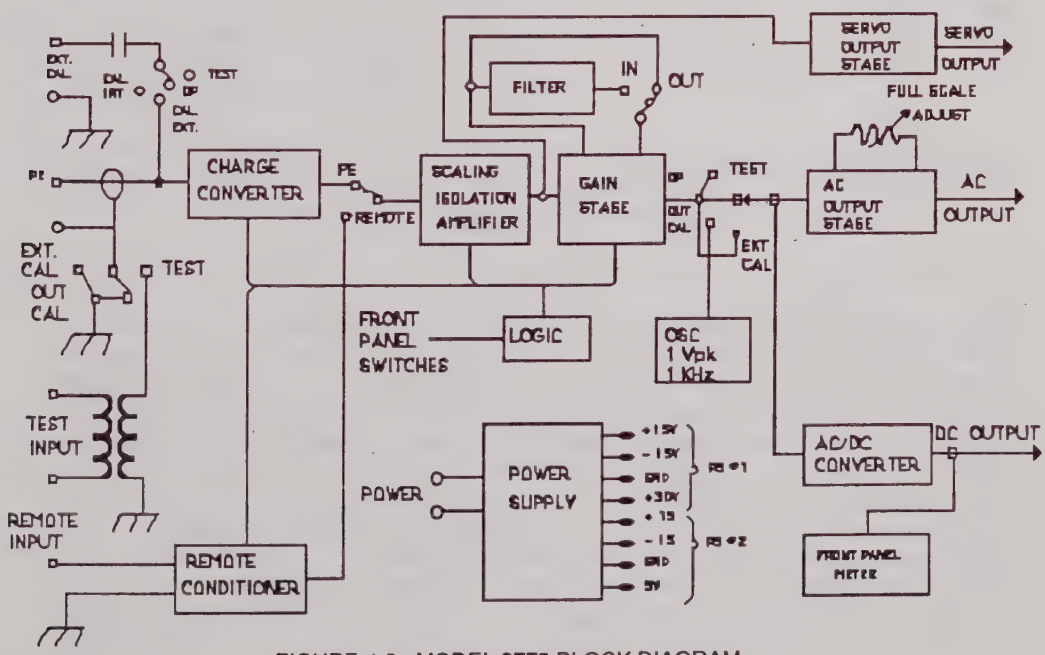

FIGURE 4-3: MODEL 2775 BLOCK DIAGRAM

A. CHARGE CONVERTER NOTE: See Schematic SC2775A

The function of the charge converter is to sense the charge applied at the PE input (J2) and to convert this charge to an analog voltage. The charge converter includes a high gain amplifier (Q3 and U3). Two different feedback capacitors establish the gain of the converter selected by a read only memory (ROM) or a programmable read only memory (PROM),on some earlier units. The gain is 1 or 0.1 mV/pC depending on the feedback capacitors (C6 or C7) connected into the circuit by the ROM switching logic. The charge converter receives a charge in pico coulombs (pC) and converts the signal to millivolts (mV) out.

The position of the Full Scale Range (g) selector switch S1 and Sensitivity Multiplier switch S2 provides encoded addresses for a read only memory (ROM U14). The ROM, in turn, provides outputs which determine the switch on/off positions that set amplifier gains. Refer to Table 4-1 for the full scale, sensitivity, multiplier and ROM output relationships.

FULL SCALE	SENSITIVITY MULTIPLIER	ROM OUTPUTS								
		Front Panel Display					Amplifier Gain			
		D7	D6	D5	D4	D3	D2	D1	D0	ROM
		17	16	15	14	13	11	10	9	Pin#
100	.1	H	H	H	H	L	L	H	L	
300	.1	H	H	H	H	H	L	H	L	
1000	.1	L	L	L	H	L	H	H	L	
3000	.1	L	H	L	H	H	L	L	L	
10000	.1	H	L	L	H	L	H	L	L	
30000	.1	H	H	L	H	H	H	L	L	
10	1	H	L	L	L	L	L	H	H	
30	1	H	H	L	L	H	L	H	H	
100	1	H	H	H	H	L	H	H	H	
300	1	H	H	H	H	H	L	L	H	
1000	1	L	L	L	H	L	H	L	H	
3000	1	L	H	L	H	H	H	L	H	
1	10	L	L	L	L	L	L	H	H	
3	10	L	H	L	L	H	L	H	H	
10	10	H	L	L	L	L	H	H	H	
30	10	H	H	L	L	H	L	L	H	
100	10	H	H	H	H	L	H	L	H	
300	10	H	H	H	H	H	L	H	H	
1	100	L	L	L	L	L	H	H	H	
3	100	L	H	L	L	H	L	L	H	
10	100	H	L	L	L	L	H	L	H	
30	100	H	H	L	L	H	L	L	H	

TABLE 4-1: 2775A MEMORY MAP

Either one of two low frequency responses can be selected by the position of the 2 Hz -0.5 Hz (previously marked >.1 Hz) switch S4. The charge converter low frequency response can be down 5% at 0.5 Hz (-3 dB at 0.2 Hz) when switch S4 is placed at 0.5 Hz, or it can be down 5% at 2 Hz (-3 dB at 0.6 Hz) when the switch is at 2 Hz position. With switch S4 placed at 0.5 Hz, the basic feedback resistor value is either R14 or R15 (depending on the gain selected by U5A) and is in the circuit to set the low frequency response for 0.5 Hz or less. When switch S4 is placed at the 2 Hz position, it causes switch U4A to close. This permits either R13 or R12 and R19 to be placed across the feedback capacitor for the gain selected. This establishes the 2 Hz low frequency response for the charge converter.

B. PREAMP INPUT CONDITIONER NOTE: See Schematic SC2775A and Figure 4-3.

Transistor Q17 is a constant current supply for an integral electronics transducer or a remote charge converter (or a remote preamp). Potentiometer R4 and resistor R99 are biasing resistors which set the proper operating point for the circuit. The AC data signal from the remote device travels along the same wire carrying DC power to the device. R4 adjusts the constant current from .5mA to greater than 20mA and should not be adjusted higher than the current rating of preamp device.

The remote preamp device senses the charge generated by a piezoelectric transducer and converts the signal into a voltage. The AC signal from a remote preamp device (remote charge converter, preamp or Isotron transducer) is coupled through capacitor C3 to a buffer (Pin 10 of Op Amp U2A). The output of the buffer is applied to a switchable X1 or X.1 attenuator (R9 and R11) controlled by signal ISO-D1 which opens or closes switch Q2. The signal from the attenuator (X1 or X0.1) is buffered by U2C and U2D and coupled through switch U4B (actuated by S5 placed at REMOTE) to the isolation amplifier.

The positions of the front panel Full Scale Range selector switch S1 and Multiplier switch S2 provide addresses for ROM U14 which outputs the logic level (0 Vdc or 5 Vdc) commands which turn Q2 on or off. With Q2 turned off, the gain of the Op Amp U2C is X1 and that of U2D is always X1 for an overall gain of X1.

If Q2 is turned on, voltage divider action causes the gain of Op Amp U2C to be X0.1 and since U2C is still at a gain of X1, the overall gain is X0.1. The gains of this signal conditioner stage correspond to the same gains switched at the charge converter stage.

C. ISOLATION AMPLIFIER NOTE: See Schematic SC2775A and Figure 4-3

The output from the Preamp Input Conditioner is routed through contacts 14 and 16 of U4B. (The switch closure on U4B is actuated by the REMOTE position of the PE-REMOTE switch S5.) From the switch, the signal is applied through a decoupling network consisting of C10, R31 and R32, to a diode protection circuit at the input of an isolation amplifier. This protects the Isolation Amplifier from very high common mode voltages (up to 500 volts) by reducing the input voltages to levels that will not damage the amplifier. The Isolation Amplifier consists of 3 Op Amps. Op Amps U6C and U6D are high impedance buffers and U7 is a differential amplifier. Gain for the Isolation Amplifier is X1 which is set by R34/R40. The two potentiometers, R37 and R39, are set to obtain the optimum common mode rejection for the differential amplifier. Potentiometer R39 allows adjustment of the DC balance between both inputs to the differential stage. Potentiometer R37 is to adjust for AC null at 1000 Hz.

Two grounds are used in the isolation amplifier circuit. There is an input ground associated with the input circuits to the 2775A and an output ground associated with the output circuits.

These grounds can be tied together or isolated from each other by the positioning of GND-ISO switch S8 (Schematic SC2775A, Sheet 3 of 3). When the grounds are isolated from each other, common mode rejection takes place at differential amplifier U7. Signals common (in phases and amplitude) to both grounds will appear simultaneously at the inputs to the differential amplifier. These signals are considered "noise" and are nulled out. All other signals are amplified by a gain factor of X1 and sent to the Sensitivity Normalization stage at Pin 18 of U9. (When the grounds are not isolated from each other, the Isolation Amplifier functions as an amplifier stage with a gain of X1.)

D. COMMON MODE VOLTAGE DETECTOR

NOTE: See Schematic SC2775A and Figure 4-3.

Working in conjunction with the Isolation Amplifier is a Common Mode Voltage Detector which functions to alert the operator via an LED indicator that the common-mode-voltage is too high. The Common Mode Voltage Detector consists of comparators U6A, U6B which sense amplitudes above a certain level (±6 Vpk). The positive level at Pin 2 is compared with the set DC level at Pin 3. When the sensed level goes above the set level, the comparator U6A turns on Q5, which in turn lights the LED indicator CR1D for at least one second. Similarly, comparator U6B senses for high negative polarity of CMV to light the LED.

E. SENSITIVITY NORMALIZATION STAGE

NOTE: See Schematic SC2775A and Figure 4-3.

The output of the Isolation Amplifier is applied to the Sensitivity Amplifier at Pin 18 of U9. The Sensitivity Normalization stage is made up of thumbwheel switches, S6A, S6B, S6C, on the front panel and of U8A, U9A and U10A. The thumbwheel switch positions change the gain of the Sensitivity Normalization stage by a ratio expressed as:

$$\frac{10}{S}$$, where S is the dialed-in sensitivity

For example, if the dialed-in sensitivity is 1.00, this yields a gain of X10:

$$\text{Gain} = \frac{10}{1} = 10$$

If the sensitivity is set for 10.99, this yields a gain of X0.9091:

$$\text{Gain} = \frac{10}{10.99} = 0.9091$$

The three-wheel switch S6 in conjunction with gate U8A provides four digits. From this stage, the output is applied to a gain stage (voltage amplifying/scaling for AC and DC out processing) and to the servo signal processing stages.

F. GAIN STAGE NOTE: See Schematic SC2775A and Figure 4-3.

The output of the Sensitivity Normalization stage is applied to the input of the gain stage (Voltage Amplifier) at Op Amp U12C. This Op Amp provides a gain of X1 or X10 depending on ROM control signal D2. (See Table 4-2.) A D2 low state provides a X10 gain and a high state switches Q7 on for a X1 gain. A plug-in type filter (if installed) is switched in or out by switch S7. The filter can be a lowpass, highpass or bandpass type. The filtered (or unfiltered) signal is coupled by C19 to Op Amp U12D which provides a gain of X1 or X3 depending on control signal D3. With D3 in the low state, the gain is X3. Signal D3 in the high state turns switch Q8 on to provide a gain of X1. The signal is then routed by mode switch S3 through a X3.4 gain amplifier (U17A) and a X1 buffer (U17B) to the AC and DC Out circuits. This voltage at the output of the voltage amplifier (GAIN) stage is scaled to 10.2 V pk full scale.

CONTROL	SWITCH	SWITCH STATE	GAIN
D2H	Q7	On	X1
D2L	Q7	Off	X10
D3H	Q8	On	X1
D3L	Q8	Off	X3

TABLE 4-2 VOLTAGE AMPLIFIER GAIN

G. SERVO AMPLIFIER NOTE: See Schematic SC2775A and Figure 4-3.

The output of the Sensitivity Normalization stage is also applied to the input of the Servo Amplifier at buffer U10B. The Servo Amplifier maintains a 10 mV/g (or a 100 mV/g) servo output regardless of the front panel sensitivity and full scale settings for the signal conditioner. Different gain stages and voltage dividers are switched as required to keep the output scaled to 10 mV/g or 100 mV/g. (The placement of jumper W1 selects 10 or 100 mV/g scaling.) Refer to Table 4-3 for Servo Amplifier gain control information and to Table 4-1 and to schematic.

CONTROL	SWITCH	SWITCH STATE	GAIN
A6H	Q9	On	X0.1
A6L	Q9	Off	X1
D1H	Q6	On	X1
D1L	Q6	Off	X10
A8L	Q10	On	X0.1
A8H	Q10	Off	X1
D0H	Q11	On	X1
D0L	Q11	Off	X10
	W1 (Jumper)	Open	X1
	W1 (Jumper)	Closed	X10

TABLE 4-3 SERVO AMPLIFIER GAIN CONTROLS

H. AC AND DC OUTPUT STAGE NOTE: See Schematic SC2775A and Figure 4-3.

The output from buffer U17B provides a 10.2 V pk full scale signal to the output circuits. This signal voltage is applied to potentiometer A2R4 and resistor A2R5 to adjust for a 1 to 10 V pk full scale AC OUT output from buffer U17, U22.

An AC-to-DC converter consisting of U16C and D takes the 10.2 V pk full scale signal and converts it to average DC. A gain factor in the circuit scales the voltage level to provide 10 Vdc out full scale. The analog front panel meter is driven from the DC output to indicate percent of full scale .

I. INTERNAL OSCILLATOR

When switch S3B is placed at OUT CAL, the Internal Oscillator is switched on via opto-isolator U21B and Q18. A signal of fixed amplitude is routed to the output stages to provide a simulated full scale output. The Internal Oscillator is comprised of U15, U19A, U19B, U19C, U19D , U16A and U16B. The reference for the oscillator is set by the 5 V pk output of U15. The 1 kHz oscillator signal output from U16A is 5 V dc. This 5 V pk output is reduced by voltage divider R68/R65 for a 3 V pk output from buffer U16B. This output is then routed, through the OUT CAL position of switch S3B, to X3.4 Op Amp U17A for a 10.2 V pk output which is applied to the AC and DC output circuits. (When the switch is at OUT CAL, all inputs from the front end of the signal conditioner are disconnected from the output circuit.)

J. POWER SUPPLY

Power supplies No. 1 and No. 2 are identical, consequently only the operation of power supply No. 2 will be discussed to serve as a description for both. A center-tapped secondary winding of transformer T2 is used to step down the voltage for power supply No. 2. The AC voltage from the secondary winding is applied to rectifier CR34. The rectifier plus and minus voltages out of CR34 are filtered by capacitors C40 and C41 and are applied to dual polarity tracking +15 V regulator U25. Resistors R95 and R97 establish the current sensing necessary to limit the power supply output currents during an overload or short circuit condition. Voltage sensing for output voltage regulation takes place at Pins 6 and 14. Transistors Q15 and Q16 add current boost to the +outputs. Capacitors C33 and C34 filter the outputs.

Regulator U23 furnishes a regulated +5V output for logic circuits. A separate +24V power supply furnishes power to a remote device such as a Remote Charge Converter or to an Isotron transducer. The supply receives the rectified voltage from full-wave rectifier CR32. This voltage is applied to voltage regulator U1 which provides a 24V output. Resistor R101 connected between the ADJ and OUT terminals permits the regulator to function as a precision current regulator which supplies constant current for a Remote Charge Converter or IE transducer through transistor Q17.

3. SPECIFICATIONS

Specifications for the Model 2775A Signal Conditioner are contained in the data sheet located in the back of this manual.

SECTION 5
MAINTENANCE/CALIBRATION

1. MAINTENANCE

The Endevco Model 2775A Signal Conditioner is maintenance free. The calibration procedure is recommended to be performed on a six month periodic basis.

2. CALIBRATION

The 2775A is designed for minimal adjustments for calibration. The unit has four adjustment potentiometers that are the AC ADJ (A2R4), the constant current adjustment (R4) and the two common mode adjustments (R37 & R39). Selected portions of the calibration procedure can be used for troubleshooting described in paragraph 5.16.

EQUIPMENT REQUIRED

The following equipment is required for unit check-out and calibration.

DVM	True rms voltmeter with ±0.1% accuracy or better (Fluke Model 8050A or equivalent)
Oscilloscope	General purpose oscilloscope 50MHz bandwidth (Tektronix Model 2213A or equivalent)
Signal Generator	Synthesizer/Function Generator 0.1Hz to 1MHz (Hewlett Packard Model 3310A or equivalent)
Frequency Counter	General purpose frequency counter (Fluke Model 1900A or equivalent)
Capacitor	Shielded Precision Capacitor 1000 pF ±1 pF (Endevco Model 2947B-2 ±1% labeled to ±1 pF)
Bandpass Filter	2 - 20 kHz

Standard parts

Desired Component			Nearest Standard Value		
30,000 pf	±5%	capacitor	30,000 pf	±5%	
5,000 pf	±5%	capacitor	4,700 pf	±5%	
			(suggest 4,700 pF and 270 pF)		
120 Ω	±1%	1W resistor	120 Ω	±5%	1W
250 Ω	±1%	resistor	249 Ω	±1%	
3.32k Ω	±1%	resistor	3.32k Ω	±1%	
10 MΩ	±1%	resistor	10 MΩ	±5%	
1N963B	12V	zener diode			
TLO72CP		op amp			
Shielded component box			2 required		

3. INITIAL SETUP

A. Remove the top cover by removing the four screws on the top of the unit. On the front panel, (Figure 5-1) set the following controls as indicated:

SENSITIVITY switch (S6) to 10.00
MULTIPLIER switch (S2) to 1
FULL SCALE switch (S1) to 100
FUNCTION switch (S3) to OP
FILTER switch (S7) to OUT
INPUT LO switch (S8) to GND
LO FREQ switch (S4) to 2Hz

B. On the back panel (Figure 5-2) set the INPUT MODE switch (S5) to PE.

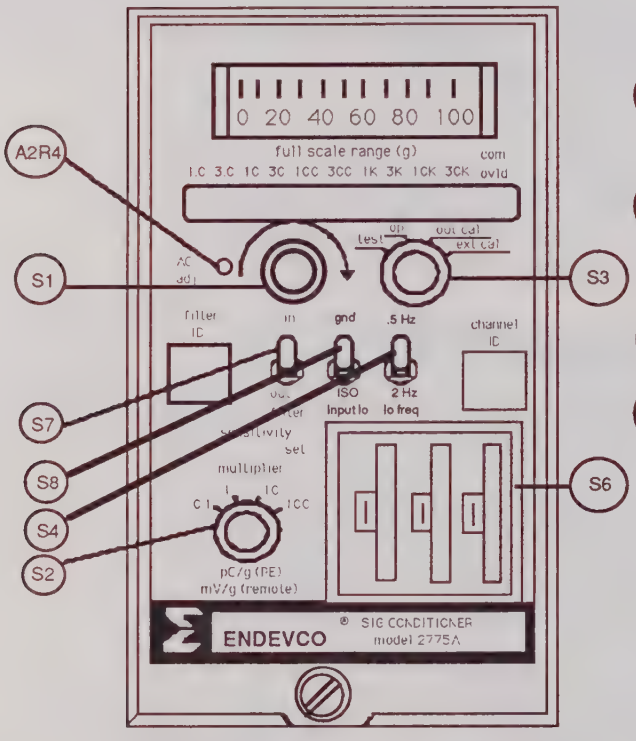

FIGURE 5-1: FRONT PANEL CONTROLS

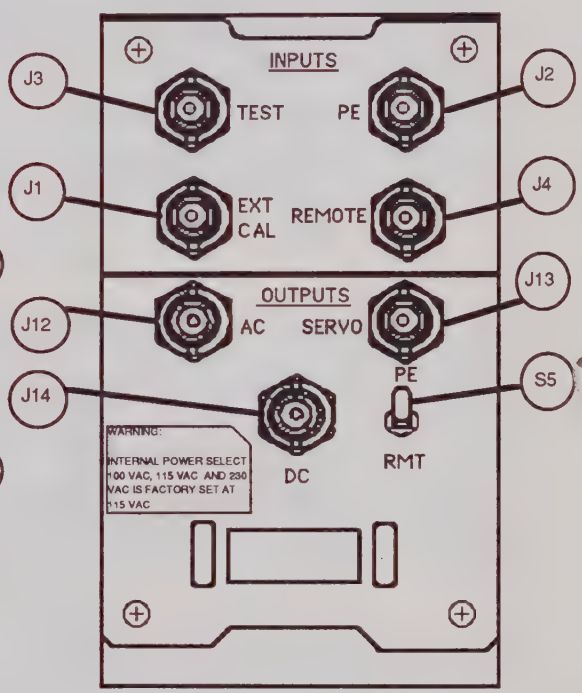

FIGURE 5-2: REAR PANEL CONTROLS

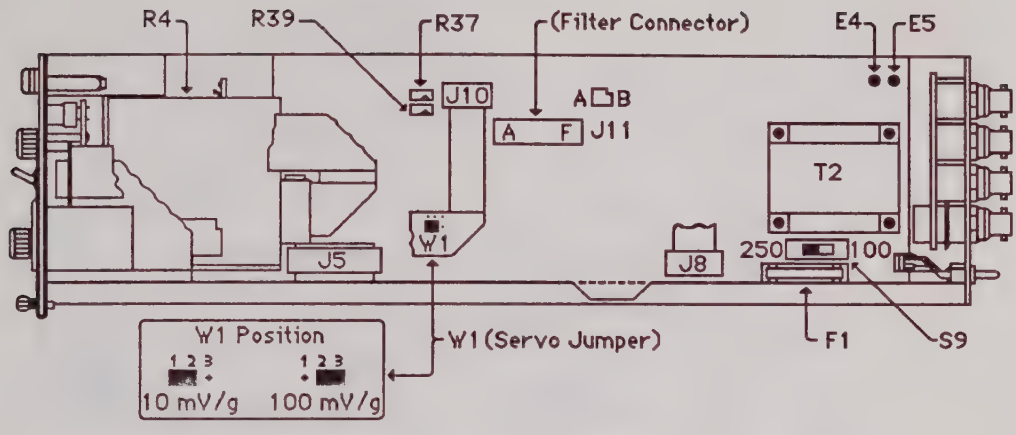

FIGURE 5-3: INTERNAL CONTROLS

C. Insure the LINE INPUT SWITCH (S9), located on the main circuit board, is set to proper line voltage. (The unit is factory set for 110Vac). Apply power and check the regulated power supplies for the proper voltages (see Figure 5-4). This unit contains two independent isolated + 15 Volt supplies

+24 Vdc +7%(gnd#1)	+5 Vdc +6%(gnd#2)
+15 Vdc +6% #1	+15 Vdc +6% #2

NOTE: Power supply #1 must be measured with respect to input ground (ground #1). Connect ground side of meter to EXT CAL (J1) shell for power supply #1 measurements. Power supply #2 must be measured with respect to output ground (ground #2) Connect ground side of meter to AC output (J12) for power supply #2 measurements.

NOTE: If the test equipment used has floating inputs, the output ground and chassis ground must be connected to avoid 60 Hz pick-up. The connection can be made on the circuit board at E4 and E5 or use a jumper from an output connector shell to the chassis. This is important for proper reading of noise and low level signals.

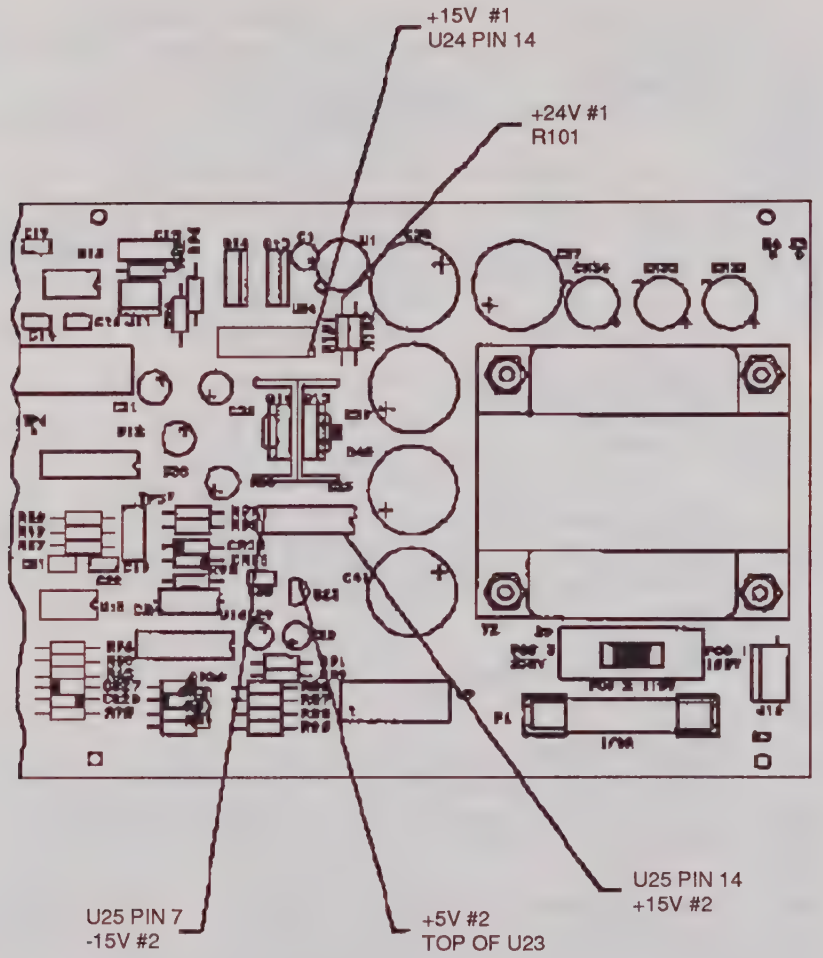

FIGURE 5-4: POWER SUPPLY TEST POINTS

4. OUTPUT CAL

A. Set INPUT LO switch to GND, FUNCTION switch to OUT CAL and monitor the AC OUTPUT (J12) with a frequency counter to verify a frequency between 950 and 1050 Hz. Monitor the DC OUTPUT (J14) for 10.0 Vdc ± 150 mVdc (see figure 5-5).

B. Monitor the AC OUTPUT with a DVM in the ac rms mode. The output level should be 7.07 Vrms ± 70 mV adjustable by the front panel AC ADJ (A2R4). Adjust the AC ADJ ccw to greater than 7.07 Vrms and then cw to less than 0.707 Vrms, this verifies the operation of the AC ADJ potentiometer. Set the AC ADJ for .707 Vrms + 1% for the next step.

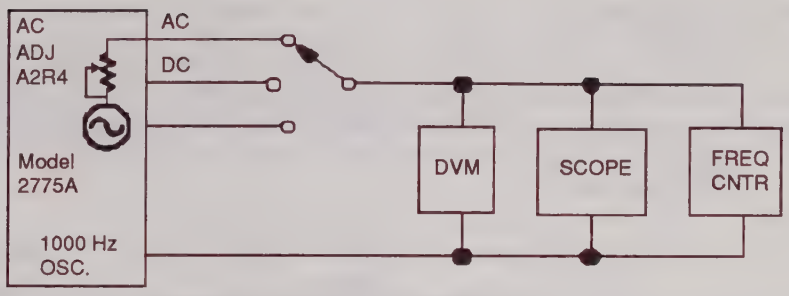

FIGURE 5-5: OUTPUT CALIBRATION

5. COMMON MODE VOLTAGE

A. With the AC ADJ adjusted for 1Vpk full scale, set the FUNCTION switch to OP and the INPUT switch to ISO. Connect a shielded 1000 pf capacitor to the PE input and ground the capacitor input to the shield of the capacitor. Connect a 100 Hz 4.242 Vrms sine signal across ground #1 (the shield of 1000 pf capacitor) and ground #2 (the outer shell of the DC OUTPUT) using ground #2 as signal common. Measure the output voltage at the AC OUTPUT using a DVM in the ac mode and monitor the signal with the oscilliscope. The maximum common mode voltage is 4.24 mVrms. (See Figure 5-6).

B. Change the frequency to 1000 Hz at the same input level and measure the AC OUTPUT for a maximum common mode voltage of 4.24 mVrms. If the common mode is high, set full scale switch to 10, and the SENSITIVITY switch to 1.00, and adjust R37 and R39 for a minimum peak to peak signal on the oscilliscope, then take the reading at 1000 Hz (see figure 5-3) and recheck the reading at 100 Hz. The adjustments of R37 and R39 are interactive and may require more than one readjustment.

C. Increase the common mode input voltage to 6.0 Vrms and observe the front panel COM OVLD LED indicator lights up. Remove the input signal and place the INPUT LO switch to GND and observe the COM OVLD LED turns off in about one second.

NOTE: Switch the INPUT LO switch into the GND position for the remaining tests.

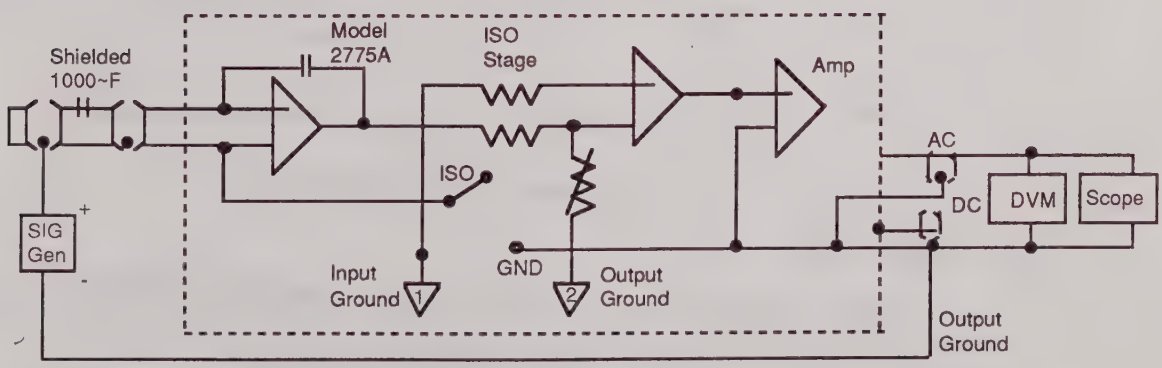

FIGURE 5-6: COMMON MODE

6. TEST INPUT

VERIFY AC ADJ adjusted for 1V pk full scale with function switch set to OUT CAL. Set the FUNCTION switch to TEST and SENSITIVITY switch to 1.00. Connect a shielded 1000 pf ±1% capacitor across the PE INPUT and apply a 70.7 mVrms 1 KHz signal to the TEST INPUT. Set the FULL SCALE switch to 100 and measure the AC OUTPUT using a DVM for approximately a full scale output.

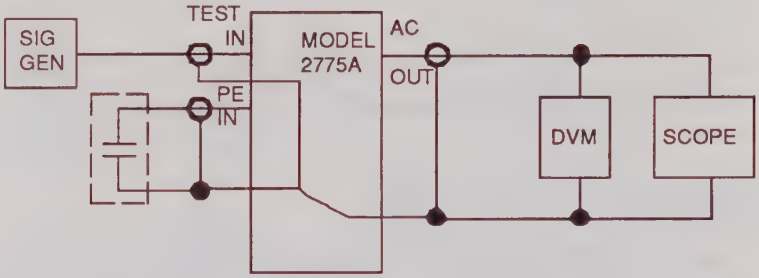

FIGURE 5-7: TEST INPUT

7. EXTERNAL CAL INPUT

NOTE: This step must be done for calibration accuracy.

Set the FUNCTION switch to OUT CAL and the FULL SCALE switch to 1K. Measure the ac amplitude at U17 pin 7, and adjust the AC ADJ for exactly this ac reading times 0.9852 at the AC OUT. Set the FUNCTION switch to EXT CAL and apply a 0.707 Vrms 1 Khz signal to the EXT CAL INPUT (J1). Measure the AC and SERVO OUTPUT (J12,J13) for a 7.07 V rms ±2 % reading. Keep present setup for the next test.

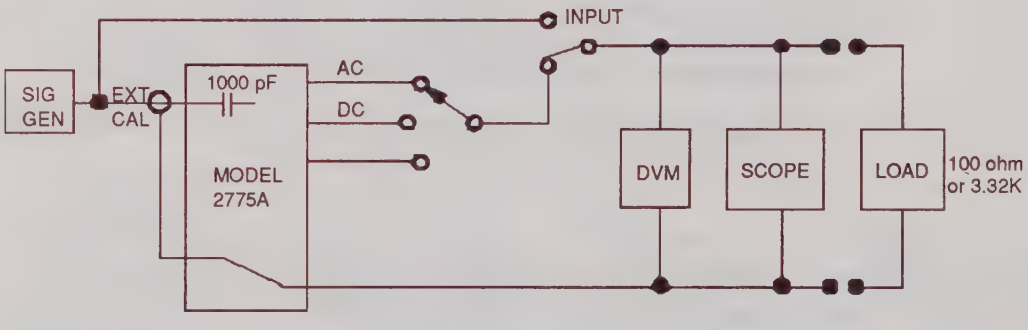

FIGURE 5-8: EXTERNAL CALIBRATION

8. MAX I OUT

A. Measure and record the full scale AC OUTPUT, SERVO OUTPUT, and DC OUTPUT voltages.

B. Connect a 120 ohm 1 watt resistor across the AC OUTPUT and measure the voltage, then compare the the loaded reading to the unloaded reading. The difference between the two readings should be less than 1%.

C. Connect a 3.32K ohm resistor across the SERVO OUTPUT and compare the voltage to the first reading. The difference between the two readings should be less than 1 %.

D. Connect the 3.32K ohm resistor across the DC OUTPUT and measure the DC voltage to compare to the first reading. The difference between the two readings should be less than 1%.

9. NOISE

Set the FULL SCALE switch to 10 and the FUNCTION switch to OP. Place a non-shorting cap on the PE INPUT. Measure the following outputs through a 2Hz to 20KHz bandpass filter. Be sure to disconnect/disable signal applied to EXT CAL input prior to noise test and place a non-shorting cap at EXT CAL also, (see Figure 5-9).

	NOISE
AC OUTPUT	15 mV rms max
SERVO OUTPUT	2 mV rms max
METER READING	Must be less than 1% deflection

A. DC OFFSET

Set the FULL SCALE switch to 3K and the FUNCTION switch to OP. Place a non-shorting cap on the PE INPUT. Measure the following outputs:

	DC OFFSET
AC OUTPUT	20 mVdc max
SERVO OUTPUT	17 mVdc max
DC OUTPUT	30 mVdc max

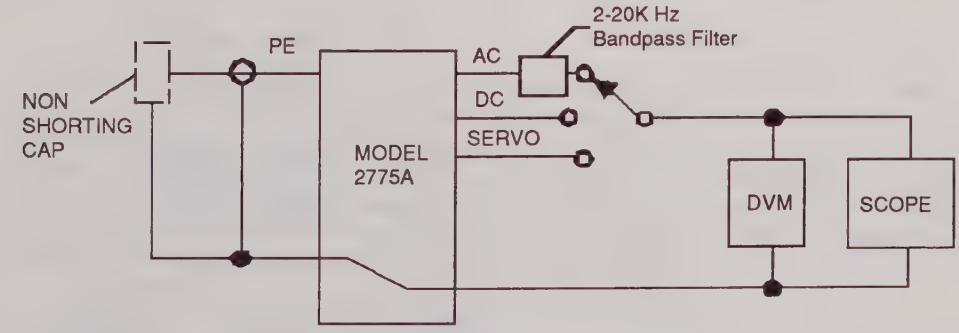

FIGURE 5-9: NOISE

10. GAIN ACCURACY

NOTE: For gain accuracy, the AC ADJ must be calibrated as follows:

1) Set the FUNCTION switch to OUT CAL.
2) Adjust AC OUT for exactly the measured ac amplitude at U17 times .9852. Set FUNCTION switch to OP.

Remove the cap from the PE INPUT and connect a 1 KHz sine signal through the shielded 1000 pF ±1pF capacitor to the PE INPUT (see figure 5-10). The EXT CAL input can be used if a precision capacitor, (figure 5-8), is not available, but the accuracy becomes ±2% (6.93-7.21 Vrms). The accuracy is ±2% because of the ±0.5% accuracy of the calibration capacitor. Set the input levels corresponding to the FULL SCALE switch and MULTIPLIER switch settings, according to the following:

INPUT mV rms	MULTIPLIER switch	FULL SCALE switch	AC OUTPUT limits
2121.0	0.1	30K	6.96-7.18 Vrms
2121.0	1	3K	6.96-7.18 Vrms
2121.0	10	300	6.96-7.18 Vrms
2121.0	100	30	6.96-7.18 Vrms
707.0	0.1	10K	6.96-7.18 Vrms
707.0	1	1K	6.96-7.18 Vrms
707.0	10	100	6.96-7.18 Vrms
707.0	100	10	6.96-7.18 Vrms

INPUT mV rms	MULTIPLIER switch	FULL SCALE switch	AC OUTPUT limits	SERVO OUTPUT limits
212.1	0.1	3K	6.96-7.18 Vrms	
212.1	1	300	6.96-7.18 Vrms	
212.1	10	30	6.96-7.18 Vrms	
212.1	100	3	6.96-7.18 Vrms	
70.7	0.1	1K	6.96-7.18 Vrms	6.96-7.18 Vrms
70.7	1	100	6.96-7.18 Vrms	696.-718. mVrms
70.7	10	10	6.96-7.18 Vrms	69.6-71.8 mVrms
70.7	100	1	6.96-7.18 Vrms	6.96-7.18 mVrms
21.21	0.1	300	6.96-7.18 Vrms	
21.21	1	30	6.96-7.18 Vrms	
21.21	10	3	6.96-7.18 Vrms	
7.07	0.1	100	6.96-7.18 Vrms	
7.07	1	10	6.96-7.18 Vrms	
7.07	10	1	6.96-7.18 Vrms	

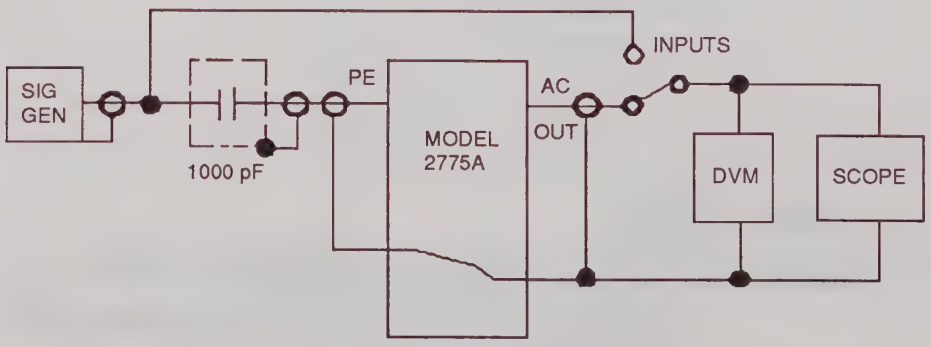

FIGURE 5-10: GAIN ACCURACY

11. SENSITIVITY SWITCH TEST

Use the previous setup and set FULL SCALE switch to 100, set the MULTIPLIER switch to 1 and input a 1 KHz signal with the value corresponding to the SENSITIVITY switch setting.

INPUT mV rms	SENSITIVITY switch	AC OUTPUT limits
141.42	2.00	6.96-7.18 Vrms
282.84	4.00	6.96-7.18 Vrms
424.26	6.00	6.96-7.18 Vrms
565.68	8.00	6.96-7.18 Vrms
707.10	10.00	6.96-7.18 Vrms
777.11	10.99	6.96-7.18 Vrms

12. FREQUENCY RESPONSE

A. The low frequency response must be measured using an oscilloscope or a special low frequency measurement device (such as a Solartron 1250 Frequency Response Analyzer). Set the SENSITIVITY switch to 1.00 and the FUNCTION switch to OUT CAL and adjust the AC OUTPUT for 1.000 Vrms. Set the FUNCTION switch to OP and adjust the signal input level to the 1000 ±1 pF shielded capacitor to read 1.00 Vrms at the AC OUTPUT. Adjust the frequency and make the following readings; see set up in Figure 5-11.

LO FREQ switch	INPUT frequency	PER CENT deviation
0.5 Hz	1 kHz	REF.
0.5 Hz	0.5 ±0.1 Hz	-5%
0.5 Hz	0.2 Hz	-3dB MAXIMUM
2 Hz	1.7-2.6 Hz	-5%
2 Hz	0.5 Hz	-3dB MAXIMUM

B. The high frequency roll off is determined by the full scale range selected in combination with the multiplier. Set the AC OUTPUT to 1.00 Vrms at 1 KHz for the reference frequency point. Increase the frequency until the AC OUTPUT drops to the -5% point and record the frequency, next increase the frequency until the AC OUTPUT drops to the - 30% (-3dB) point and record the frequency. Readjust the AC OUTPUT reference to 1.00 Vrms at 1 KHz for each full scale range. The frequency recorded should be greater than the frequency listed for each full scale range. (See Figure 5-11 for Setup).

FULL SCALE switch	AC OUTPUT reference	AC OUTPUT -5% point	AC OUTPUT -30% point
10	1 KHz	25 kHz	75 kHz
30	1 KHz	30 kHz	90 kHz
100	1 KHz	40 kHz	120 kHz
300	1 KHz	30 kHz	90 kHz
1K	1 KHz	50 kHz	150 kHz
3K	1 KHz	50 kHz	150 kHz

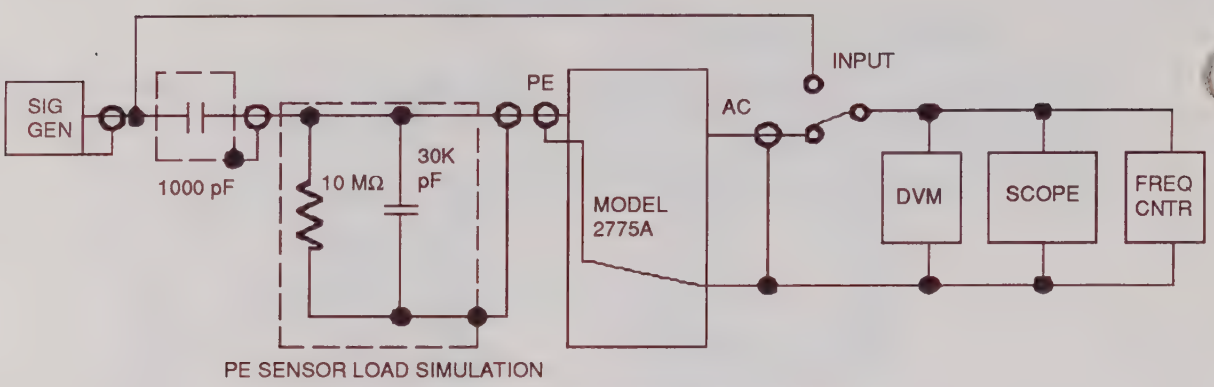

FIGURE 5-11: FREQUENCY RESPONSE

13. REMOTE GAIN ACCURACY

Set the FUNCTION switch to OUT CAL and the FULL SCALE switch to 3K. Measure the ac amplitude at U17 pin 7 and adjust the AC ADJ for exactly this ac reading times .9852 at the AC OUT. Set the FUNCTION switch to OP and set the back panel MODE switch to RMT and connect a 1 KHz sine signal through the current blocking circuit (fig 5-12) to the REMOTE INPUT (J4). Set the MUTIPLIER switch to 1 and set the FULL SCALE switch per the following table.

INPUT mV rms	FULL SCALE switch	AC OUTPUT limits
2121.0	3k	6.96-7.18 Vrms
707.0	1K	6.96-7.18 Vrms
212.1	300	6.96-7.18 Vrms
70.7	100	6.96-7.18 Vrms
21.21	30	6.96-7.18 Vrms
7.07	10	6.96-7.18 Vrms

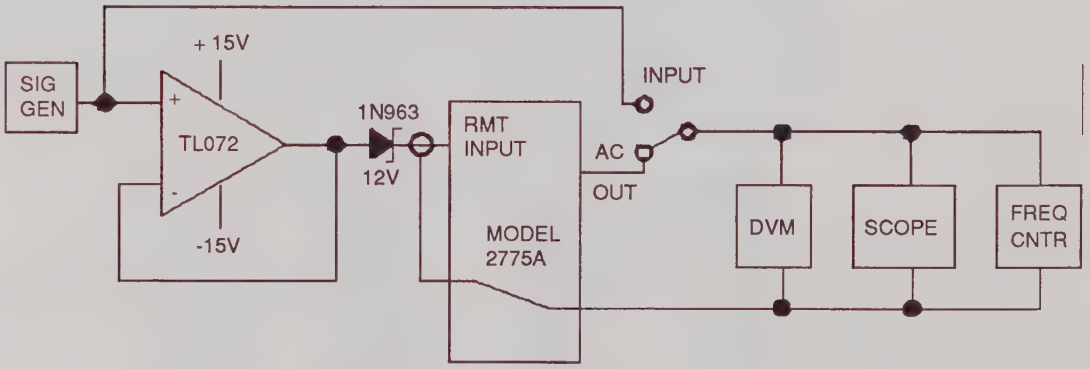

FIGURE 5-12: REMOTE GAIN

14. REMOTE FREQUENCY RESPONSE

A. The low frequency response must be measured using an oscilloscope or a special low frequency measurement device (such as a Solartron 1250 Frequency Response Analyzer). Use the previous setup. Set the FULL SCALE switch to 100 and set the FUNCTION switch to OUT CAL and adjust the AC OUTPUT for 1.000 Vrms. Set the FUNCTION switch to OP and adjust the input level to read 1.000 Vrms at the AC OUTPUT. Adjust the frequency and make the following readings; (Same set-up as Figure 5-12).

INPUT frequency	PER CENT deviation
1 KHz	REF.
0.5 Hz	>-5%
0.2 Hz	>-3dB

B. The high frequency roll off is determined by the full scale range selected in combination with the multiplier. Set the AC OUTPUT to 1.00 V rms at 1 KHz for the reference frequency point. Increase the frequency until the AC OUTPUT drops to the -5% point and record the frequency, next increase the frequency until the AC OUTPUT drops to the - 30% (-3dB) point and record the frequency. Readjust the AC OUTPUT reference to 1.00 Vrms at 1 KHz for each full scale range. The frequency recorded should be greater than the frequency listed for each full scale range (Figure 5-12).

FULL SCALE switch	AC OUTPUT reference	AC OUTPUT -5% point	AC OUTPUT -30% point
10	1 KHz	24 KHz	70 KHz
30	1 KHz	24 KHz	70 KHz
100	1 KHz	30 KHz	90 KHz
300	1 KHz	35 KHz	100 KHz
1K	1 KHz	70 KHz	190 KHz
3K	1 KHz	70 KHz	190 KHz

15. REMOTE NOISE

Remove the input signal from the REMOTE INPUT and connect a 250 ohm resistor and a 5000 pf capacitor in parallel across the REMOTE INPUT. Set the FULL SCALE switch to 10. Be sure the REMOTE constant current source is set to 4ma dc. The bandwidth of the rms noise measurement is 2 Hz to 20 KHz.

NOISE	
AC OUTPUT	5 mV rms max
SERVO OUTPUT	2 mV rms max
METER READING	Must be less than 2% deflection

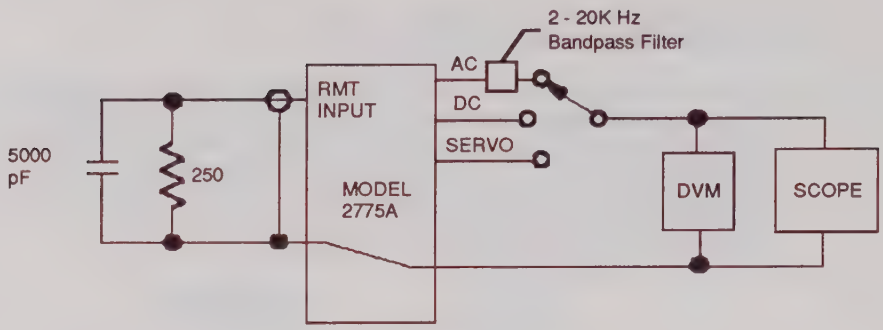

FIGURE 5-13: REMOTE NOISE

16. CONSTANT CURRENT ADJUST

Connect a DVM in the DC current mode to the REMOTE INPUT (J4). Adjust the constant current adjust R4 through the hole in the shield on the main circuit board (see figure 5-4) for a range of 0.5 mA to 20 mA. The current is factory set at 4 mA for Isotron accelerometer operation, but should be set for operational requirements (see 3.4.13) if other devices or long input lines are used. If the 2771A remote charge converter is used the current should be set to 10 mA.

NOTE: R4 can be adjusted to greater than 20 mA which could damage Isotron accelerometers. Do not leave current adjusted higher than 20 mA.

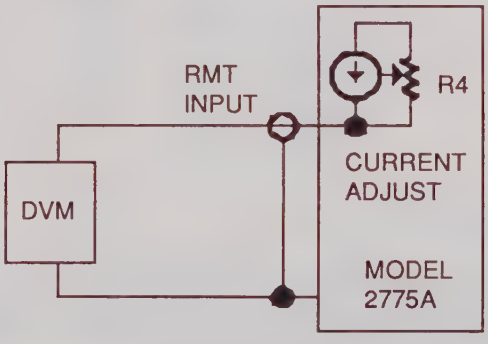

FIGURE 5-14: CONSTANT CURRENT ADJUST

17. TROUBLESHOOTING GUIDE

Symptoms	Checks
No indicator LEDs on any range	1. Check power cord and line power. 2. Check fuse F1 on main circuit board. 3. Check power supply voltages see section 5.2.3
LEDs out on some ranges	1. Check U20 and replace if faulty.

	2. Check U14 logic IC. See table 4-1.
LEDs on, but no output	1. Set FUNCTION switch to OUT CAL and check AC OUTPUT. See paragraph 5.3.
No OUT CAL signal at AC OUTPUT	1. Check U17 & U22 output stage 2. Check U16 oscillator output see paragraph 4.2.9
OUT CAL signal good, but no signal output.	1. Set FILTER switch to OUT and check for signal. if the filter jumper is installed the FILTER switch has no effect. 2. Perform Ext Cal test paragraph 5.6.
Ext Cal test good, but no signal output.	1. Check input cable to the PE INPUT for continuity and proper hookup 2. Check accelerometer for correct capacitance & resistance readings 3. Perform the TEST function see paragraph 3.4.5.
PE operation good, but no REMOTE signal output	1. Insure the remote input device is a constant current type i.e. Isotron accelerometer or remote 2. Check the REMOTE INPUT see paragraph 5.12 & 5.15
No output with REMOTE or PE input.	1. Check isolation stage of the unit, refer to paragraph 4.2.3 2. Check the gain stage of the unit, refer to paragraph 4.2.6
REMOTE operation good, but PE operation bad	1. Check charge converter section, refer to paragraph 4.2.1
Line frequency noise on the output signal.	1. Check for ground loops in the system see paragraph 2.4.3 2. Insure the EXT CAL INPUT has a shorting cap or is connected to a low impedance source such as a function generator. 3. Check that the output ground is connected to third wire ground through external equipment or install a jumper at E4 & E5 on the circuit board paragraph 2.2.3.
Output readings appear too high or low.	1. Check AC ADJ paragraph 5.3.2. 2. Check gain accuracy paragraph 5.9.

	3. Perform the SENSITIVITY switch test paragraph 5.10. 4. Verify accelerometer calibration
AC OUTPUT readings good but the meter reading is off.	1. Check the DC OUTPUT by the OUT CAL test paragraph 5.3.1. 2. Check meter and connections.

18. REPAIR

Access to component parts and sub-assemblies is gained by removal of the unit's top cover. Further disassembly and re-assembly for repair is easily accomplished. Section 7 provides part location diagrams and parts lists for electrical components. Standard good workmanship practices should be employed for removal and replacement of components.

19. FACTORY SERVICE

If serious trouble occurs, and the instrument cannot be adjusted or repaired to meet specifications, return the amplifier to the factory. It should always be accompanied by a detailed statement describing the fault noted.

Endevco warrants each new instrument to be free from defects in material and workmanship for one year from the date of sale to the original purchaser. This warranty does not extend to units that have been mistreated, used in violation of Endevco recommendations, or to units that have been altered or repaired outside of Endevco's factory. Defects covered by this warranty will be corrected at no charge when the unit is delivered to the factory with all transportation charges prepaid. If, upon examination, it is found that a defect is not within the scope of this warranty, a statement of repair charges and a request for authorization to proceed with repair will be submitted to the purchaser.

See the complete warranty enclosed with this manual. Address all shipments and correspondence to:

Endevco
Technical Services Dept.
30700 Rancho Viejo Rd.
San Juan Capistrano. CA
92675

SECTION 6
OPTIONS AND ACCESSORIES

1. ACCESSORIES INCLUDED

The following accessory items are included with the Model 2775A:

QTY	ITEM
1	17180 Power Cord Assembly or 17180V Power Cord Assembly for 230-volt line power.
1	BNC to MICRODOT (10-32 thread) Adaptor Plug, Endevco P/N EJ21. This adapter plug permits the use of a cable with a Microdot 10-32 thread connector.

2. ACCESSORIES AVAILABLE

The following accessories for use with the Model 2775A are available from Endevco:

Model 2771A-X Remote Charge Converter	Converts high impedance pC charge input to a low impedance mV output. Three gain ranges are available; X= 0.1, 1 or 10.
Model 4948 Rack Adapter (6-channel)	Houses from one to six Model 2775A Signal Conditioners. Each signal conditioner plugs into a power receptacle at the rear of the rack adapter. Individual signal conditioners are held in place on the adapter by the knurled captive screw mounted on the front panel. Blank panels, P/N 16678, may be used to cover vacant slots. A power switch on the front panel applies power to all signal conditioners in the adapter. The Model 4948 is designed to fit a 19-inch rack cabinet.
Blank Panels P/N 16678	Blank panels for covering empty channel slots in the Model 4948 Rack Adapter.
Adjustable Filter Card P/N 35771	Plug-in type filter for processing of data signals. Adjustable to act as a high-pass, low-pass, or bandpass filter. Has selectable cut-off frequencies.

3. ADJUSTABLE FILTER

An adjustable filter card, P/N 35771, is available for use in the Model 2775A. This plug-in filter card is adjustable by moving a DIP programming jumper to form two high-pass, seven low-pass, or a bandpass filter from any combination of high-pass and low-pass filters on the card. The card also includes two unpopulated resistor positions for customer installation (or factory ordered installation) of filters with customized frequencies. The filters are active type, 2-pole Butterworth and are non-inverting in phase. The selectable cut-off frequencies for the adjustable filter are:

HP Cut-Off Frequencies -5%	LP Cut-Off Frequencies -5%
Custom	Custom
2 Hz	100 Hz
10 Hz	200 Hz
500 Hz	
	1000 Hz
	2000 Hz
	5000 Hz
	10 000 Hz

A. FILTER PROGRAMMING

A low-pass, high-pass, or bandpass filter can be programmed. To program a low-pass (LP) filter or a high-pass (HP) filter on the Programmable Filter Card:

1. Place a DIP jumper at the proper position to select the mode, i.e., LP (low-pass) or HP (high-pass). (See Figure 6-1).
2. Install another jumper to select the desired high-pass or low-pass cut-off (corner) frequency. (See Figure 6-1).

To program a bandpass (BP) filter:

1. Place a DIP jumper at the BP position to select the bandpass mode.
2. Install two jumpers to select a cut-off frequency from the low-pass (LP) filter section and a cut-off frequency from the high-pass (HP) filter section. (See Figure 6-1).

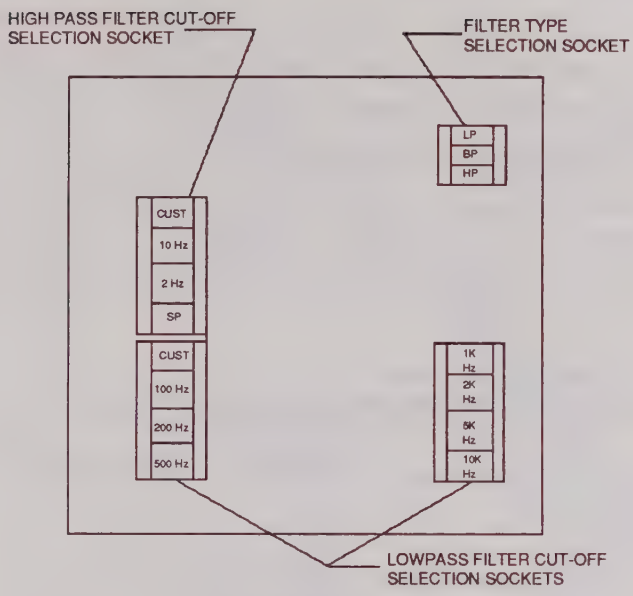

FIGURE 6-1: PROGRAMMING JUMPER SELECTION

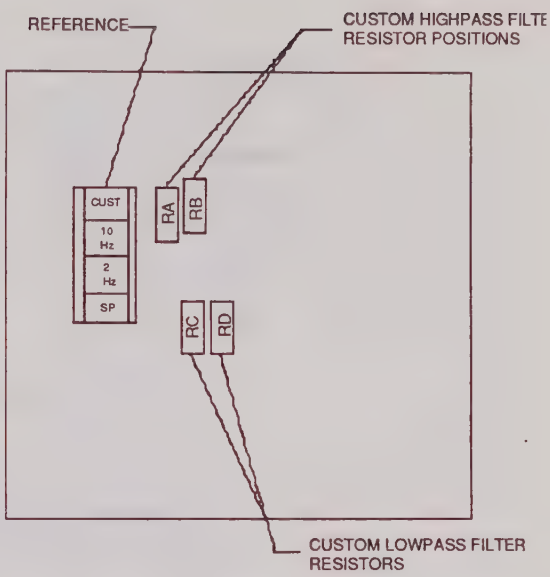

FIGURE 6-2: CUT-OFF RESISTOR POSITIONS

B. SELECTING CUSTOM HIGH-PASS CUT-OFF FREQUENCIES.

Cut-off frequencies for a 2 Hz to 200 Hz high-pass filter range can be selected. To establish a desired -5% cut-off (corner) frequency for a customized high-pass, 2-pole Butterworth filter:

1. Select a desired cut-off frequency and, using Figure 6-3, first determine the resistance value of resistors RA.

2. Double the value of RA to find the resistance value of RB, that is, RB = 2RA.

3. Use the calculated resistance values of RA and RB to make resistor selections that match (as closely as possible) the resistance of commonly available 1%, 1/10 W standard resistors.

4. Install the resistors. (See Figure 6-2 for resistor locations).

C. SELECTING CUSTOM LOW-PASS CUT-OFF FREQUENCIES.

Cut-off frequencies for a 100 Hz to 20 kHz low-pass filter range can be selected. To establish a desired -5% cut-off (corner) frequency for a customized low-pass, 2-pole Butterworth filter:

1. Select a desired cut-off frequency and, using Figure 6-4, first determine the resistance value of resistors RC and RD. Both are the same in value (RC = RD).

2. Use the value to select resistors that match (as closely as possible) the resistance of commonly available ±1%, 1/10 W standard resistors.

3 Install the resistors. (See Figure 6-2 for resistor locations).

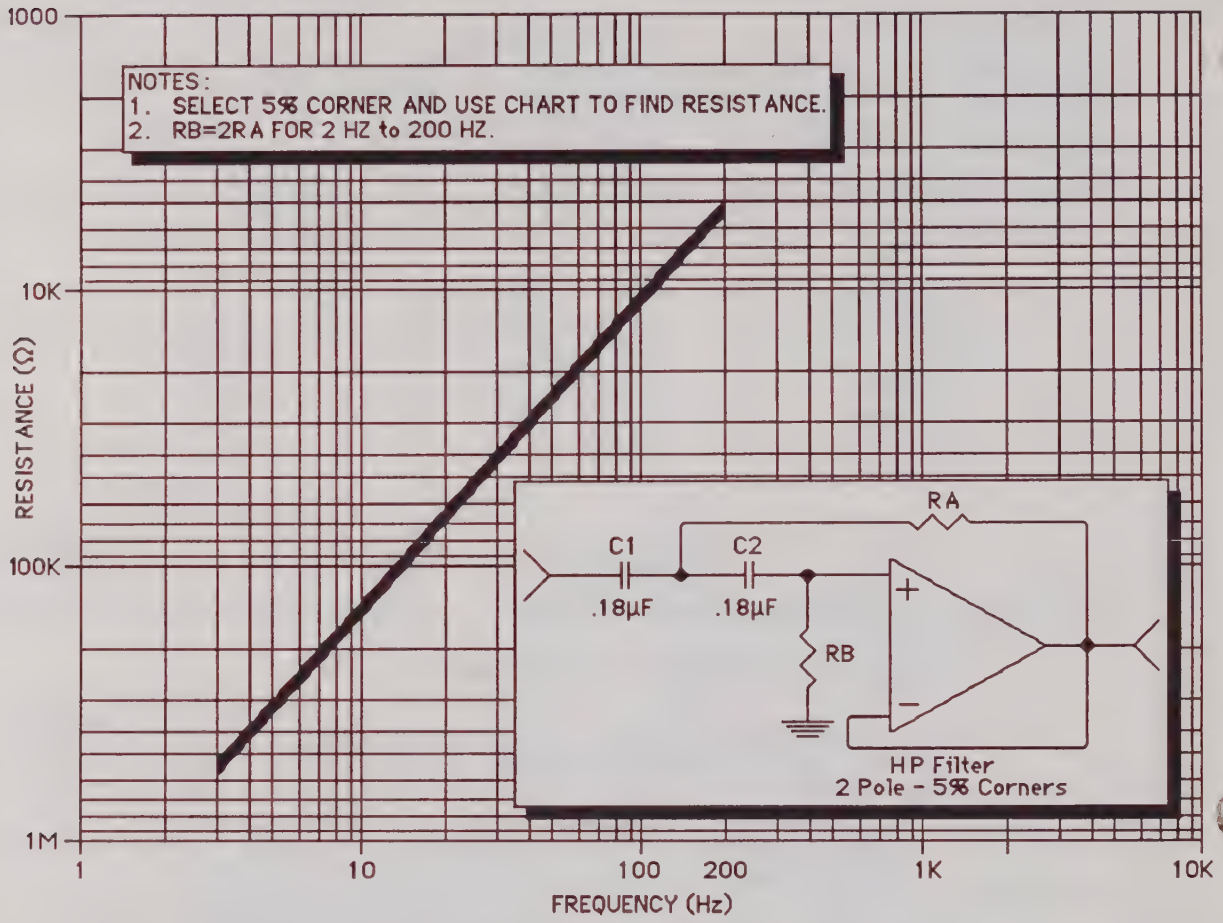

FIGURE 6-3: HIGH-PASS RESISTOR SELECTION CHART

NOTES:

1. Three DIP programming jumpers are provided for user installation as needed. Two jumpers are always used, and the third is used only when a bandpass filter is selected.

2. When only a high-pass or a low-pass filter is selected, the third programming jumper may be stored in the SP (spare) position.

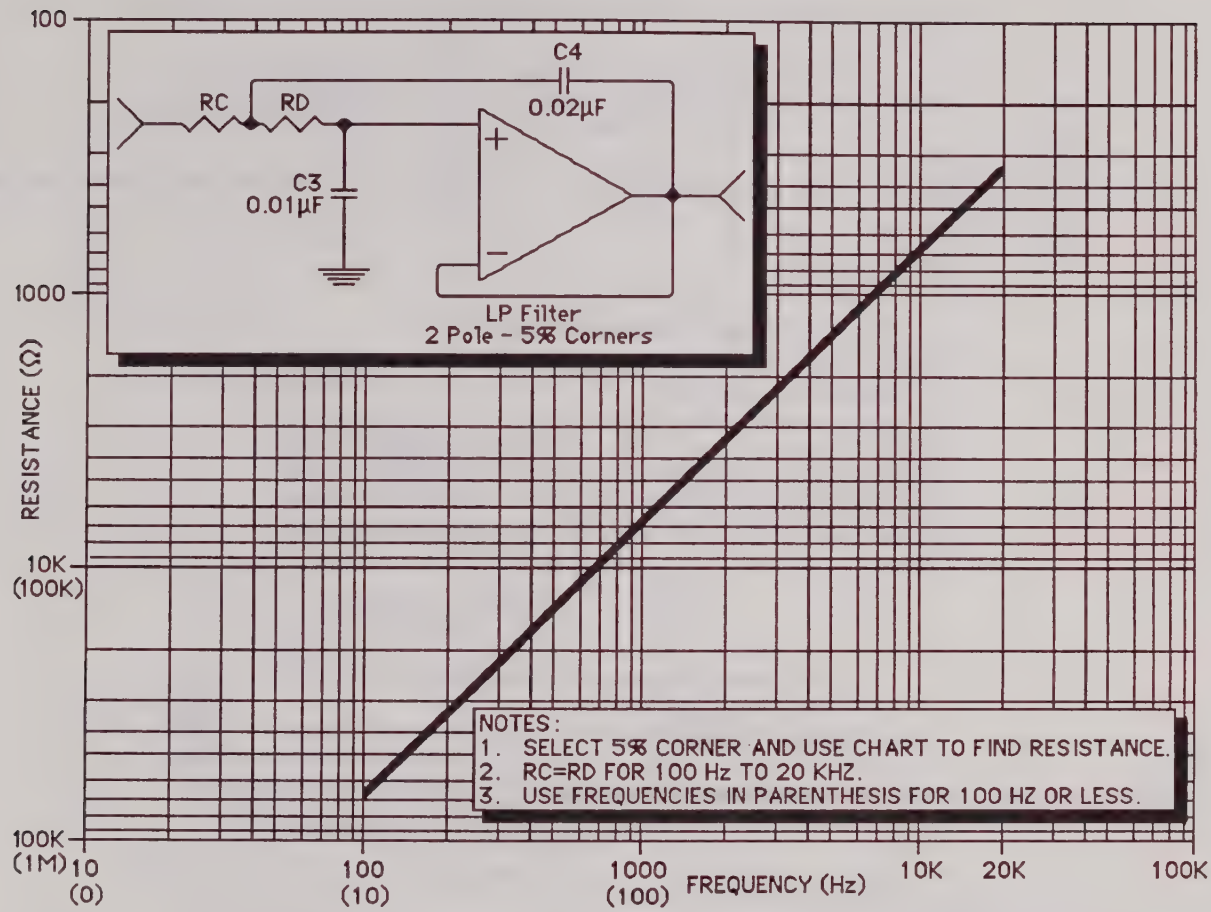

FIGURE 6-4: LOW-PASS RESISTOR SELECTION CHART

The Model 2771A-X remote charge converter (RCC) is an electronic device that converts the signal from a high impedance PE device to a low impedance voltage source. The RCC can be placed close to transducer at a remote location to drive long lines through hostile electrical environments with far less noise pick-up than would be possible with high impedance sources. Endevco RCCs use a two wire system that allows both power and signal to transmitted on the same line.

The Model 2775A provides the constant current power source at the REMOTE input to the unit adjustable from 0.5mA to 20mA. The 2771A requires a minimum of 4mA to 20mA for proper operation. There are frequency and voltage limitations when driving extremely long lines see section 3.4.13 for remote input interface factors.

There are three gain ranges for the Model 2771A-X RCC and they are as follows:

2771A-01 attenuation of 0.1 mV/pC +1% -2%
2771A-1 unity gain of 1 mV/pC +1% -2%
2771A-10 gain of 10 mV/pC +1% -5% marked with gain

NOTE: The 2771A is an inverting device. The output is 180 degrees out of phase with the input.

A. KEY FEATURES

Up to 30,000 pF source capacitance
Operates down to 100 K ohm source resistance
10 V pk-pk output minimum
Wide frequency response 1Hz to 50KHz (-01 & -1) -3dB @ 0.2Hz
(-10) frequency response of 5Hz to 50KHz -3db @ 1Hz
Wide temperature range -40 C to +100 C
10-32 input connector and BNC output connector
Rugged construction, cold rolled steel case hot solder dipped

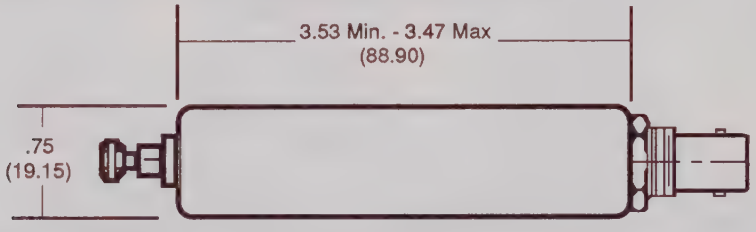

FIGURE 6-5: 277A DIMENSIONS

B. 2771A TESTING WITH THE 2775A

The 2771A RCC with the 2775A Signal Conditioner comprises a system. The system gain accuracies are a combination of the two devices. The 2771A-01/-1 converters are rated at +1% -2% and the 2775A is rated at ±1.5% accuracy. The system gain accuracy would be +2.5% and -3.5% un-calibrated. The accuracy and tolerances of the test setup and equipment must also be considered. The following procedure for checking the Model 2771A may be used for incoming inspection and for periodic calibration. The 2771A must be tested with a Model 2775A or other properly rated constant current source.

C. TEST EQUIPMENT

Refer to the equipment list on page one of section 5. Hook up the equipment in accordance with figure 6-6.

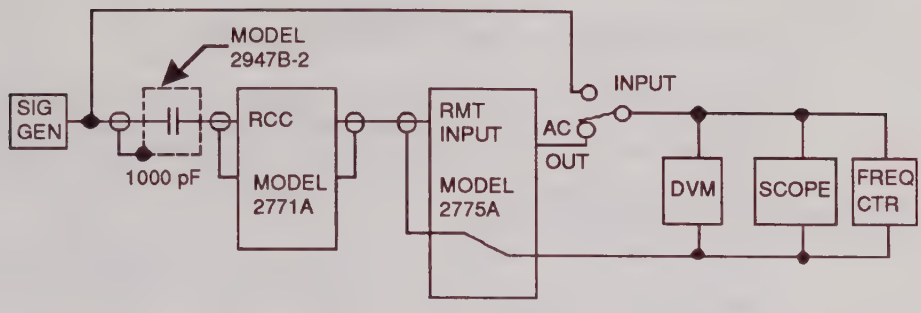

FIGURE 6-6: 2771A/2775A TEST SETUP

D. INITIAL CONDITONS

2775A SETUP	
Sensitivity switch to	- 1.00 (enter actual -10 gain)
Sensitivity multiplier	- x.1(-01),x1(-1),x10(-10)
Full scale g	- 1Kg
Function	- OP
Filter	- OUT
Input isolation	- GND
LO freq	- 2Hz
Set AC output to 1Vpk	

NOTE: For best gain accuracy, the AC ADJ must be calibrated as follows:
1) Set FUNCTION switch to OUT CAL.
2) Adjust AC OUT for exactly one-tenth the measured ac amplitude at U17 pin 7. Set the FUNCTION switch to OP.

E. FULL SCALE RANGE TEST 2771A-1

Apply a 1KHz 707mV rms (1Vpk) Sine signal through the 1000pF capacitor to the input of the RCC. The 2775A AC output should be 707mV rms undistorted sine within +2.5% & -3.5% of the input.

Switch the full scale range to 100g and decrease the input signal to 70.7mV rms. The AC output should be 707mV rms +2.5% -3.5%.

Switch the full scale range to 10g and decrease the input signal to 7.07mV rms. The AC output should be 707mV rms +2.5% -3.5%.

F. NOISE TEST

Reduce the input to zero by turning off the oscillator or by grounding the input to the capacitor. Measure the noise at the 2775A AC output with the true rms voltmeter. The noise should be less than 15mV rms broadband noise with 1000pF source capacitance.

G. FREQUENCY RESPONSE

Set the full scale switch to 1000g and adjust the input for 707mV at the 2775A AC output. Change the oscillator frequency from 2Hz to 50kHz referenced to 1kHz with a tolerance of ±5%. The 2771A-10 is 5Hz to 50kHz ±5%.

H. 2771A UNIT GAIN ACCURACY TEST

Apply a 1kHz 707mV rms sine signal through the capacitor to the RCC input. Measure the RCC output from a BNC tee connector with a DVM. The output voltage should be 707mV rms +1% -2%. This value is the actual gain tolerance of the 2771A unit. (see Figure 6-7).

I. BIAS VOLTAGE CHECK

Change the DVM to read DC volts and measure the DC bias voltage of the 2771A. The bias voltage should be between +9V and +11V DC at room temperature and between +8V and +12V DC over -40 C to +100 C.

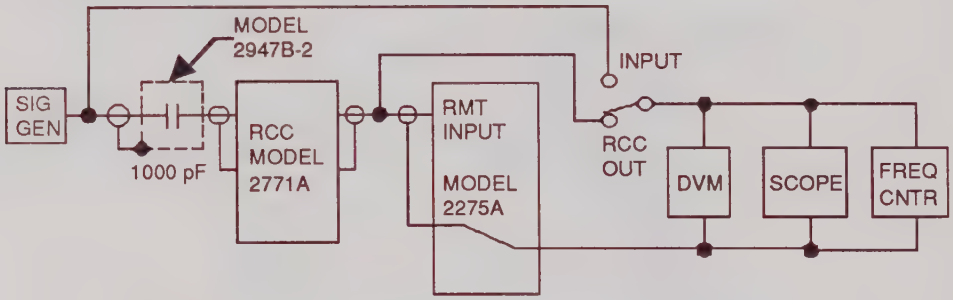

FIGURE 6-7: 2771A GAIN AND BIAS SETUP

SECTION 7
DRAWINGS AND PARTS LISTS

1. GENERAL

This section includes drawings of the amplifier and the rack adapter (accessory item). Schematic drawings and electrical parts lists are in this section. Other applicable drawings and reference documents are also included.

2. PARTS LISTS

The followings parts lists (which are keyed to the assembly drawings) are contained in this section:

Parts List	
Signal Conditioner Circuit Board Assembly	PL26469
Rear Panel Circuit Board Assembly	PL26476
Front Panel Circuit Board Assembly	PL26563
Signal Conditioner Final Assembly	PL92775A

3. DRAWINGS

The following schematics and assembly drawings are in this section:

Description	
Signal Conditioner	92775A
Signal Conditioner Circuit Board Assembly	26469
Front Panel Circuit Board Assembly	26563
Rear Panel Circuit Board Assembly	26476
Signal Conditioner Schematic Diagram	SC2775A
Rack	4948-C
Rack Adapter Schematic	4948-501C

ENDEVCO 2775A
INSTRUCTION MANUAL

Calibration Check Sheet

Date:_____ 2775A Serial No._____

Power Supply

	+24 Vdc ±7%	_____	+5 Vdc ±6%	_____
No. 1	+15 Vdc ±6%	_____	-15 Vdc ±6%	_____
No. 2	+15 Vdc ±6%	_____	-15 Vdc ±6%	_____

Out Cal

Frequency 950-1050 Hz _____
DC OUTPUT 10.00 Vdc ±150 mVdc _____
AC ADJ (A2R4) ccw greater than 7.07 Vrms _____
AC ADJ (A2R4) cw less than .707 Vrms _____

Common Mode

100 Hz 4.24 mVrms(max)_____ 1 KHz 4.24 mVrms(max) _____
If reading is high adjust R37 & R39 at 1 KHz for minimum
levels and recheck at 100 Hz.
the COM OVLD LED turns on with 6.0 Vrms (Y/N) _____
COM OVLD LED should turn off in one second(Y/N) _____

Test Input Check for a full scale output of approximately .707 Vrms.

Ext Cal Input AC OUTPUT 6.93-7.21 Vrms _____
SERVO OUTPUT 6.93-7.21 Vrms_____

Max Current Out

_____ AC OUTPUT no load_____ Vrms with load_____ Vrms 1% max.
_____ SERVO OUTPUT no load_____ Vrms with load_____ Vrms 1% max.
_____ DC OUTPUT no load_____ Vrms with load_____ Vrms 1% max.

Noise/DC Offset

AC OUTPUT 15 mVrms max_____ DC offset 20 mVdc max._____
SERVO OUTPUT 2 mVrms max _____ DC offset 17 mVdc max._____
DC OUTPUT - DC offset 30 mVdc max._____
METER READING less than 2%

NOTE: The PE INPUT and EXT CAL INPUT must be capped with a non-shorting cap.

PE Gain Accuracy

Accuracy will be ±1.5% using shielded 1000 ±1pF capacitor
Accuracy will be ±2.0% using the EXT CAL INPUT for calibration.

limits ±1.5% = 6.96-7.18 Vrms
limits ±2.0% = 6.93-7.21 Vrms

INPUT mVrms	FULL SCALE switch	AC OUTPUT reading	INPUT mVrms	FULL SCALE switch	AC OUTPUT reading	SERVO reading
2121.0	30K	_____	707.0	10K	_____	
2121.0	3K	_____	707.0	1K	_____	
2121.0	300	_____	707.0	100	_____	
2121.0	30	_____	707.0	10	_____	
212.1	3K	_____	70.7	1K	_____	_____
212.1	300	_____	70.7	100	_____	_____
212.1	30	_____	70.7	10	_____	_____
212.1	3	_____	70.7	1	_____	_____
21.21	300	_____	7.07	100	_____	
21.21	30	_____	7.07	10	_____	
21.21	3	_____	7.07	1	_____	

Sensitivity Switch Test

SENSITIVITY switch	AC OUTPUT reading
2.00	_____
4.00	_____
6.00	_____
8.00	_____
10.00	_____
10.99	_____

PE Frequency Response

	1 KHz	-5%	-30%
Low Freq .5 Hz deviation	ref	_____Hz	_____Hz
2 Hz deviation	ref	_____Hz	_____Hz
High Freq FULL SCALE 10	ref	_____KHz	_____KHz
FULL SCALE 30	ref	_____KHz	_____KHz
FULL SCALE 100	ref	_____KHz	_____KHz
FULL SCALE 300	ref	_____KHz	_____KHz
FULL SCALE 1K	ref	_____KHz	_____KHz
FULL SCALE 3K	ref	_____KHz	_____KHz

Remote Gain Accuracy

FULL SCALE switch	AC OUTPUT reading
3K	_____ Vrms
1K	_____ Vrms
300	_____ Vrms
100	_____ Vrms
30	_____ Vrms
10	_____ Vrms

Remote Frequency Response

	1 KHz	-5%	-30%
Low Freq 0.5 Hz deviation	ref	_____ Hz	_____Hz
High Freq FULL SCALE 10	ref	_____ KHz	_____KHz
FULL SCALE 30	ref	_____ KHz	_____KHz
FULL SCALE 100	ref	_____ KHz	_____KHz
FULL SCALE 300	ref	_____ KHz	_____KHz
FULL SCALE 1K	ref	_____ KHz	_____KHz
FULL SCALE 3K	ref	_____ KHz	_____KHz

Remote Noise

AC OUTPUT 5mVrms max_____
SERVO OUTPUT 2 mVrms max_____
METER READING less than 2% _____

Note: REMOTE INPUT must be loaded with 250 ohm resistor and a 5000 pf capacitor in parallel.

Constant Current Adjust

Minimum current less than 0.5mA_____ mA
Maximum current greater than 20mA____ mA
Constant current set to:_____ mA

Notes:

ENDEVCO
San Juan Capistrano, Ca

PARTS LIST Dwg No PL92775A

Title: Signal Conditioner

dwg	chkd	appr	sht	date	rev	eo no
WM 07-09-84	PQ 11-17-84	GB 10-18-84	1 of 3	09-21-92	AP	20311

Item	Ind	Part No	Rev	Description	Qty
		SC2775A	-	Signal Conditioner	-
		PL26469	W	PCB Assy, Signal Conditioner	-
		PL26563	D	PCB Assy, Front Panel	-
		PL26476	B	PCB Assy, Rear Panel	-
		PL26480	C	PCB Assy, Thumbwheel Switch	-
		VD26560	A	Version Description Document (Gain/Disply Data	-
		FD26560	A	Flexible Disk (Program)	-
		SL26560	A	Source Listing (Program)	-
	1	92775A	L	Signal Conditioner	1
1	2	26441	D	Case, Lower	1
2	2	26442	D	Case, Upper	1
3	2	26456	C	Mounting Bar	2
	3	26810-3213	-	Al 2024-T351 .375 sq	16"
4	2	EW99	-	Tape, Teflon	1.5"
5	-	---	-	Not Used	-
6	-	---	-	Not Used	-
7	2	25950	C	Panel, Front, Molded	1
8	2	26542	B	Metal-Cal, I.D.	1
	3	AW26542	A	Metal-Cal, I.D.	1
	2	26481	C	Label, Front Panel	1
	3	AW26481	C	Label, Front Panel	1
10	2	26482	B1	Panel, Rear	1
	3	26482-98	-	Panel, Fabricated and Anodized	1
	4	26482-99	-	Panel, Fabricated	1
	3	AW26482	C	Panel, Rear	1
11	2	26539	D	Shield, Lower	1
	3	26539-99	-	Shield, Lower, Fabricated	1
	3	EHM867	-	Standoff, Swage	4
12	2	26538	C	Shield, Upper	1
	3	26538-99	-	Shield, Upper, Fabricated	1
	3	EHM868	-	Standoff, Swage	4
13	2	26011-30	A	Twisted Pair Cable Assy	1
	3	EP436	-	Connector, Socket, 2 Pos	1
	3	EW762	-	Twisted Pair, 24 AWG, Red/Blk	8"
14	2	26469-3	J	PCB Assy, Signal Conditioner (A1)	1
15	2	26563	C	PCB Assy, Front Panel (A2)	1
16	2	26476	B	PCB Assy, Rear Panel (A3)	1
17	2	17902-62	1A	Coaxial Cable Assy (PE Input)	1
	3	EJ132	-	Connector, Coaxial	1
	3	EW104	-	Coaxial Cable	15.5"
	3	EW377	-	Solder Sleeve	1
	3	EW400	-	Wire 24 AWG Gry	1.5"
18	2	EHM736	-	Knob	2
	2	EHM739	-	Knob (Without Index Line)	1
	2	EHM330	-	Fastener	1

Item	Ind	Part No	Rev	Description	Qty
	-	---	-	Not Used	-
22	2	EH319	-	Screw, Mach FH, No. 4-40 x 3/8	6
23	3	EH200	-	Screw, Mach, Nylon 4-40 X 1/4	2
24	2	EHW104	-	Washer, Shoulder, 5/16	1
25	2	EHW173	-	Lockwasher, No. 2	10
26	2	EHM935	-	Spacer	2
	3	EHM839	-	Standoff	1
27	2	EHW105	-	Washer, 5/16	1
28	2	26040	B1	Filter Bypass Assy	1
	3	EJ240	-	Connector	1
	3	EW32	-	Wire 22 AWG Blk	1"
29	2	2970-22	B	Model Serial Plate	1
	3	AW2970-22	B	Model Serial Plate	1
30	2	EH362	-	Screw, Mach, 2-56 x 7/16	4
31	2	EHR100	-	Grommet, Caterpillar	2"
32	2	EHN111	-	Nut, 1/2-28	6
33	2	EHW260	-	Lockwasher, Internal Tooth, .5	6
34	-	---	-	Not Used	-
35	-	---	-	Not Used	-
36	2	17335-1	1A	Bracket, Mounting, Connector	1
37	2	17335-2	1A	Bracket, Mounting, Connector	1
38	2	EH476	-	Screw, Mach, 0-80 x 1/2	1
39	2	EHW171	-	Lockwasher, No. 0	1
40	2	26480-1	C	PCB Assy, Thumbwheel Switch	1
41	2	26484-20	B	Cable Assy, AC In	1
	3	EW37	-	Wire 22 AWG Blk	5"
	3	EW37	-	Wire 22 AWG Grn	5"
	3	EW35	-	Wire 22 AWG Wht	5"
	3	EP449	-	Connector, 3 Pin	1
42	-	---	-	Not Used	-
43	3	EW304	-	Cable Assy	1
44	2	26527-56	A	Cable Assy, Shielded, 10 Cond	1
	3	EP431	-	Connector Socket, 10 Pos	2
	3	EW775	-	Ribbon Cable, 10 Cond	14"
45	2	EH336	-	Screw, Mach 100deg FH, 4-40 x .250 (Blk Oxd)	12
46	2	26519-65	D	Coaxial Cable Assy (Remote)	1
	3	EJ567		Connector, Coaxial	1
	3	EW795	-	Coaxial Cable	16.2"
	3	EW377	-	Solder Sleeve	1
	3	EW480	-	Wire 24 AWG Gry	2"
47	2	EHJ317	-	Bushing, Shoulder, 1/2	1
48	2	EHW40	-	Washer, Flat, 1/2	1
49	-	---	-	Not Used	-
50	2	EHW129	-	Washer, Flat, No. 2	1
51	2	EHE54	-	Clamp, Cable	1
52	2	EH461	-	Screw, Mach PH, 2-56 X 5/16	6

Item	Ind	Part No	Rev	Description	Qty
	2	26444	B	Mounting Block	2
	3	26810-3213	-	Al 2024-T351 .375 sq	.5"
54	2	26409	B	Mounting Block	2
	3	26810-3213	-	Al 2024-T351 .375 sq	.5"
M1	2	16482	A1	Meter	1
P8	2	EJ322	-	Connector, Power	1

ENDEVCO
San Juan Capistrano, Ca

PARTS LIST Dwg No PL26469

Title: PCB Assy, Sig Cond

orig	chkd	appr	sht	date	rev	eo no
TB 09-05-84	GS 10-17-84	GB 10-18-84	1 of 7	09-21-92	W	20311

Item	Ind	Part No	Rev	Description	Qty
		SC2775A	Ref	Signal Conditioner	-
		FD26560	A	Flexible Disk (Program)	-
		SL26560	A	Source Listing (Program)	-
		VD26560	A	Version Description Document (Gain/Disply Data	-
	1	26469-X	J	PCB Assy, Signal Conditioner	1
1	2	26468	F	PCB, Signal Conditioner	1
	3	AW26468	F	PCB, Signal Conditioner	1
2	2	EHM766	-	Heat Sink	2
3	2	EHB20	-	Shoulder Bushing	2
4	2	EHN54	-	Nut, Hex, Small Pattern 4-40	5
5	2	EHW15	-	Lockwasher, Split, #4	1
6	2	EH334	-	Screw, 4-40 x 1/2	1
7	2	EH333	-	Screw, Mach, 4-40 X 3/8	4
8	2	EHW164	-	Lockwasher, Internal Tooth, No 4	4
9	2	EHW250	-	Washer, Isolating, Transistor Mtg	3
10	2	EXF12	-	Fuse Clip	2
11	2	13157-16	3E	Standoff	1
[illegible]	2	EX42	-	Socket, 24 Pin	1
[illegible]	2	EE253	-	Wire-Wrap Pin	3
14	2	EJ553	-	Polarizing Key	6
15	2	EHM1003	-	Heat Sink	1
16	2	EHX38	-	Adhesive, RTV	.1oz
C1	2	0130-105035	-	Cap Tan Elec 1uF, 35V	1
C2	2	EC1632	-	Cap 1000pF	1
C3	2	0129-105	-	Cap Cer Z5U 1uF	1
C4	2	0130-475035	-	Cap Tan Elec 4.7uF, 35V	1
C5	2	0129-105	-	Cap Cer Z5U 1uF	1
C6	2	0136-103	-	Cap .01uF	1
C7	2	0104-102F	-	Cap Mica DM15 1000pF 1% 100V RL	1
C8	2	0104-220J	-	Cap Mica DM15 22pF 5% 500V RL	1
C9	2	0129-104	-	Cap Cer Z5U .1uF	1
C10	2	0129-225	-	Cap Cer Z5U 2.2uF	1
C11	2	0130-105035	-	Cap Tan Elec 1uF, 35V	1
C12	2	0104-101J	-	Cap Mica DM15 100pF 5% 500V RL	1
C13	2	0104-220J	-	Cap Mica DM15 22pF 5% 500V RL	1
C14	2	0129-104	-	Cap Cer Z5U .1uF	1
C15	2	0129-105	-	Cap Cer Z5U 1uF	1
C16	2	0129-104	-	Cap Cer Z5U .1uF	1
C17	2	0129-104	-	Cap Cer Z5U .1uF	1
C18	2	0129-104	-	Cap Cer Z5U .1uF	1
C19	2	0129-105	-	Cap Cer Z5U 1uF	1
C20	2	0129-104	-	Cap Cer Z5U .1uF	1
[illegible]	2	0129-104	-	Cap Cer Z5U .1uF	1
C22	-	---	-	Not Used	-

Item	Ind	Part No	Rev	Description	Qty
	2	0129-105	-	Cap Cer Z5U 1uF	1
C24	2	0134-153	-	Cap Met Poly .015uF	1
C25	2	0134-153	-	Cap Met Poly .015uF	1
C26	2	0129-105	-	Cap Cer Z5U 1uF	1
C27	-	---	-	Not Used	-
C28	2	0130-106025	-	Cap Tan Elec 10uF, 25V	1
C29	2	0130-105035	-	Cap Tan Elec 1uF, 35V	1
C30	2	0129-104	-	Cap Cer Z5U .1uF	1
C31	2	0130-106025	-	Cap Tan Elec 10uF, 25V	1
C32	2	0130-106025	-	Cap Tan Elec 10uF, 25V	1
C33	2	0130-106025	-	Cap Tan Elec 10uF, 25V	1
C34	2	0130-106025	-	Cap Tan Elec 10uF, 25V	1
C35	2	0129-104	-	Cap Cer Z5U .1uF	1
C36	2	0129-104	-	Cap Cer Z5U .1uF	1
C37	2	0117-337050	-	Cap Al Elctlt 330uF, 50V	1
C38	2	0117-108035	-	Cap Al Elctlt 1000uF, 35V	1
C39	2	0117-108035	-	Cap Al Elctlt 1000uF, 35V	1
C40	2	0117-108035	-	Cap Al Elctlt 1000uF, 35V	1
C41	2	0117-108035	-	Cap Al Elctlt 1000uF, 35V	1
C42	2	0129-104	-	Cap Cer Z5U .1uF	1
C43	2	0130-226015	-	Cap Tan Elec 22uF, 15V	1
C44	2	0130-476020	-	Cap Tan Elec 47uF, 20V	1
C45	2	0130-476020	-	Cap Tan Elec 47uF, 20V	1
C46	2	0104-220J	-	Cap Mica DM15 22pF 5% 500V RL	1
C47	2	0104-102J	-	Cap Mica DM15 1000pF 5% 100V RL	1
	2	0208-11	-	Diode 1N916B	28
Thru CR28					
CR29	-	---	-	See Dash Numbers	-
CR30	2	0208-11	-	Diode 1N916B	-
CR31	2	0208-11	-	Diode 1N916B	1
CR32	2	ECR242	-	Diode Bridge, W02	1
CR33	2	ECR242	-	Diode Bridge, W02	1
CR34	2	ECR242	-	Diode Bridge, W02	1
CR35	2	0208-11	-	Diode 1N916B	1
CR36	2	0208-11	-	Diode 1N916B	1
CR37	2	ECR298	-	Diode SB030	1
CR38	2	0208-11	-	Diode 1N916B	1
F1	2	EF21	-	Fuse 1/4A Slo-Blo	1
J1	-	---	-	Not Used on This Assy	-
J2	-	---	-	Not Used on This Assy	-
J3	-	---	-	Not Used on This Assy	-
J4	-	---	-	Not Used on This Assy	-

Item	Ind	Part No	Rev	Description	Qty
J5	2	EJ554	-	Connector, 26 Pos	1
J6	2	EJ555	-	Connector, 20 Pos	1
J7	2	EJ550	-	Connector, 10 Pos	1
J8	-	---	-	Not Used on This Assy	-
J9	2	EJ550	-	Connector, 10 Pos	1
J10	2	EX69	-	Socket, 14 Pin	1
J11	2	EJ556	-	Connector, 2 Pos	1
J12	-	---	-	Not Used on This Assy	-
J13	-	---	-	Not Used on This Assy	-
J14	-	---	-	Not Used on This Assy	-
J15	2	EP243	-	Connector, 6 Pin	1
J16	2	EJ576	-	Connector, 3 Pos	1
K1	2	EK89	-	Relay	1
K2	2	EK88	-	Relay	1
Q1	2	0404-3904	-	XSTR 2N3904	1
Q2	2	EQ487	-	Fet, J109	1
Q3	2	EQ970	-	LS844-71 Dual JFET	1
Q4	2	EQ230	-	XSTR MPS-A13	1
Q5	2	EQ487	-	Fet, J109	1
Q6	2	EQ485	-	FET J112	1
Q7	2	EQ487	-	Fet, J109	1
Q8	2	EQ487	-	Fet, J109	1
Q9	2	EQ782	-	FET J110	1
Q10	2	EQ782	-	FET J110	1
Q11	2	EQ485	-	FET J112	1
Q12	-	---	-	See Dash Numbers	-
Q13	2	EQ817	-	XSTR TIP29AFP	1
Q14	2	EQ817	-	XSTR TIP29AFP	1
Q15	2	EQ817	-	XSTR TIP29AFP	1
Q16	2	EQ817	-	XSTR TIP29AFP	1
Q17	2	0404-2905	-	XSTR 2N2905	1
Q18	2	EQ487	-	Fet, J109	1
R1	2	0305-244	-	Res 240K	1
R2	2	0305-513		Res 51K	1
R3	-	---	-	Not Used	-
R4	2	ER2827	-	Pot Trim PCB 1K	1
R5	2	0305-220	-	Res 22ohm	1
R6	2	0305-475	-	Res 4.7M	1
R7	2	0305-512	-	Res 5.1K	1
R8	2	0306-151	-	Res 150ohm	1
R9	2	0329-9092	-	Res 90.9K	1
R10	-	---	-	Not Used	-

Item	Ind	Part No	Rev	Description	Qty
R11	2	0329-1012	-	Res 10.1K	1
R12	2	0305-626	-	Res 62M	1
R13	2	0305-366	-	Res 36M	1
R14	2	0305-916	-	Res 91M	1
R15	2	0305-108	-	Res 1000M	1
R16	2	0309-3652	-	Res 36.5K	1
R17	2	0309-3652	-	Res 36.5K	1
R18	2	0305-105	-	Res 1M	1
R19	2	0305-307	-	Res 300M	1
R20	2	0305-103	-	Res 10K	1
R21	2	0329-1002	-	Res 10K	1
R22	2	0305-103	-	Res 10K	1
R23	2	0329-1002	-	Res 10K	1
R24	2	0305-106	-	Res 10M	1
R25	2	0309-1373	-	Res 137K	1
R26	2	0309-1373	-	Res 137K	1
R27	2	0309-1053	-	Res 105K	1
R28	2	0309-1053	-	Res 105K	1
R29	2	0309-3652	-	Res 36.5K	1
R30	2	0309-4992	-	Res 49.9K	1
R31	2	0309-4992	-	Res 49.9K	1
R32	2	0305-115	-	Res 1.1M	1
R33	2	0305-105	-	Res 1M	1
R34	2	0329-1002	-	Res 10K	1
R35	2	0329-1002	-	Res 10K	1
R36	2	ER3434	-	Res SIP 7 X 150K	1
R37	2	ER2941	-	Pot 100K	1
R38	2	0309-9761	-	Res 9.76K	1
R39	2	ER2368	-	Pot 500ohm	1
R40	2	0329-1002	-	Res 10K	1
R41	2	ER3434	-	Res SIP 7 X 150K	1
R42	2	0305-116	-	Res 11M	1
R43	2	0329-1012	-	Res 10.1K	1
R44	2	0309-1371	-	Res 1.37K	1
R45	2	0309-1371	-	Res 1.37K	1
R46	2	0329-9092	-	Res 90.9K	1
R47	2	0329-1012	-	Res 10.1K	1
R48	2	0329-1002	-	Res 10K	1
R49	2	0329-9092	-	Res 90.9K	1
R50	2	0329-2002	-	Res 20K	1
R51	2	0329-9091	-	Res 9.09K	1
R52	2	0309-1003	-	Res 100K	1
R53	2	0309-1003	-	Res 100K	1
R54	2	0329-1001	-	Res 1K	1
R55	2	0309-3652	-	Res 36.5K	1
R56	2	0309-3652	-	Res 36.5K	1

Item	Ind	Part No	Rev	Description	Qty
[illegible]	2	0305-116	-	Res 11M	1
R58	2	ER3434	-	Res SIP 7 X 150K	1
R59	2	0329-9091	-	Res 9.09K	1
R60	2	0329-1001	-	Res 1K	1
R61	2	0329-1012	-	Res 10.1K	1
R62	2	0329-9092	-	Res 90.9K	1
R63	2	0329-3402	-	Res 34K	1
R64	2	0329-1153	-	Res 115K	1
R65	2	0329-2402	-	Res 24K	1
R66	2	0305-244	-	Res 240K	1
R67	2	0305-513	-	Res 51K	1
R68	2	0329-1602	-	Res 16K	1
R69	2	0305-116	-	Res 11M	1
R70	2	0309-6040	-	Res 604ohm	1
R71	2	0329-1011	-	Res 1.01K	1
R72	2	0329-9091	-	Res 9.09K	1
R73	2	0329-9091	-	Res 9.09K	1
R74	2	0309-1072	-	Res 10.7K	1
R75	2	0309-1072	-	Res 10.7K	1
R76	2	0309-1072	-	Res 10.7K	1
R77	2	0305-394	-	Res 390K	1
R78	2	0305-116	-	Res 11M	1
R79	2	0309-1072	-	Res 10.7K	1
R80	-	---	-	See Dash Numbers	-
R81	2	0309-1001	-	Res 1K	1
[illegible]	-	---	-	See Dash Numbers	-
R83	2	0329-2002	-	Res 20K	1
R84	2	0329-1002	-	Res 10K	1
R85	2	0309-4992	-	Res 49.9K	1
R86	2	0316-150	-	Res 15, 1W, Wire Wound, 5%	1
R87	2	0329-1002	-	Res 10K	1
R88	2	0329-1002	-	Res 10K	1
R89	2	0329-1102	-	Res 11.0K	1
R90	2	0329-1102	-	Res 11.0K	1
R91	2	0329-2002	-	Res 20K	1
R92	2	0309-1001	-	Res 1K	1
R93	2	0309-1003	-	Res 100K	1
R94	2	0305-2R7	-	Res 2.7ohm	1
R95	2	0305-2R7	-	Res 2.7ohm	1
R96	2	0305-2R7	-	Res 2.7ohm	1
R97	2	0305-2R7	-	Res 2.7ohm	1
R98	-	---	-	See Dash Numbers	-
R99	2	0309-8451	-	Res 8.45K	1
R100	2	0305-101	-	Res 100ohm	1
R101	2	0309-5490	-	Res 549ohm	1
R102	2	0309-9761	-	Res 9.76K	1

Item	Ind	Part No	Rev	Description	Qty
R103	2	0305-107	-	Res 100M	1
R104	2	0305-204	-	Res 200K	1
R105	2	0305-472	-	Res 4.7K	1
R106	2	0305-390	-	Res 39 ohm	1
R107	2	0305-390	-	Res 39 ohm	1
S9	2	ES282	-	Switch, Slide, 3P3T	1
T1	2	ET39	-	Transformer	1
T2	2	26687	C	Transformer, Power	1
TP1	2	EE253	-	Wire-Wrap Pin	1
TP2	2	EE253	-	Wire-Wrap Pin	1
TP3	2	EE253	-	Wire-Wrap Pin	1
TP4	2	EE253	-	Wire-Wrap Pin	1
TP5	2	EE253	-	Wire-Wrap Pin	1
TP6	2	EE253	-	Wire-Wrap Pin	1
U1	2	EQ752	-	LM317H	1
U2	2	EQ474	-	TL074CN	1
U3	2	EQ478	-	NE5534AN	1
U4	2	EQ643	-	LF130202N	1
U5	2	EQ751	-	DG243CJ	1
U6	2	EQ474	-	TL074CN	1
U7	2	EQ478	-	NE5534AN	1
U8	2	EQ432	-	CD4002BE	1
U9	2	EQ647	-	AD7525KN	1
U10	2	EQ484	-	TL072CP	1
U11	2	EQ474	-	TL074CN	1
U12	2	EQ474	-	TL074CN	1
U13	2	0503-43	-	TL064C	1
U14	-	---	-	See Dash Numbers	-
U15	2	EQ750	-	REF02HP	1
U16	2	0503-42	-	TL074BCN	1
U17	2	EQ474	-	TL074CN	1
U18	2	EQ650	-	MC14504BCP	1
U19	2	EQ474	-	TL074CN	1
U20	2	EQ649	-	MC14051BCP	1
U21	2	EQ612	-	MCT6	1
U22	2	EQ645	-	LH0002CH	1
U23	2	EQ652	-	LM78L05CZ	1
U24	2	EQ543	-	LM325N	1
U25	2	EQ543	-	LM325N	1
U26	2	EQ652	-	LM78L05CZ	1
W1	2	EW789	-	Jumper, Mini	1

Item	Ind	Part No	Rev	Description	Qty
		For -1 Assy			
CR29	2	0208-11	-	Diode 1N916B	1
Q12	2	0404-3904	-	XSTR 2N3904	1
R80	2	0305-472	-	Res 4.7K	1
R82	2	0305-472	-	Res 4.7K	1
R98	2	0305-474	-	Res 470K	1
U14	2	26560-1	C	IC, Programmed	1
	3	EQ648	-	HM3-6641-5	1
		For -2 Assy			
CR29	-	---	-	Not Used	-
Q12	-	---	-	Not Used	-
R80	-	---	-	Not Used	-
R82	-	---	-	Not Used	-
R98	2	0305-681	-	Res 680ohm	1
U14	2	26560-2	C	Programmed (U14)	1
		For -3 Assy			
CR29	-	---	-	Not Used	-
Q12	2	EW23	-	Wire 24 AWG Solid	.5*★
R80	-	---	-	Not Used	-
R82	-	---	-	Not Used	-
R98	2	0305-681	-	Res 680ohm	1
U14	2	26560-3	C	IC, Programmed	1
	3	EQ818	-	NMC27C32Q-45	1

★ Bus Wire to Jumper Emitter & Collector position

ENDEVCO

San Juan Capistrano, Ca.

IMPORTANT NOTICE: INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO CONFIDENTIAL. REPRODUCTION, DUPLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY.

FSCM 95411

PARTS LIST

ORIG	CHKD	APPR	TITLE	REV	DATE	EO. NO.	SHEET	
WM DATE 07/06/84	GS/PQ DATE 10/17/84	GB DATE 10/18/84	CIRCUIT BOARD ASSEMBLY REAR PANEL	B	04/22/85	16062	1/2	PL26476

ITEM NO.	SIZE	IND NO.	DWG NO./PART NO.	CUST DWG	REV	EO. NO.	DESCRIPTION	QTY
			CONTROL DWG					
	A		PL26476A		-	-	CIRCUIT BOARD ASSEMBLY, REAR PANEL (PARTS LIST)	-
	D		SC2775A	*	-	REF		
	C	1	26476		B	16062	CIRCUIT BOARD ASSY, REAR PANEL	1
1	C	2	26475		B	16062	CIRCUIT BOARD, REAR PANEL	1
		3	AW26475		B	16062	ARTWORK, REAR PANEL	-
C1		2	0129-104			-	CAPACITOR, .1µF	1
C2		2	0129-104				CAPACITOR, .1µF	1
J1			EJ546				RECEPTACLE, BNC	1
J3			EJ546				RECEPTACLE, BNC	1
J12			EJ546				RECEPTACLE, BNC	1
J13			EJ546				RECEPTACLE, BNC	1
J14			EJ546				RECEPTACLE, BNC	1
J18			EJ550				HEADER, 10 PIN	1
J19			EJ550				HEADER, 10 PIN	1

.NEEVCO PARTS LIST

SHEET 2

PL26576

ITEM NO.	SIZE	IND NO.	DWG NO./PART NO.	CUST DWG	REV	EO. NO.	DESCRIPTION	QTY
R1		2	0309-4991				RESISTOR, 4.99K	1
R2		2	0309-4991				RESISTOR, 4.99K	1
S5		2	ES234				SWITCH, TOGGLE, SPDT	1

IMPORTANT NOTICE: INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO CONFIDENTIAL. REPRODUCTION, DUPLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY.

ENDEVCO
San Juan Capistrano, Ca.

FSCM 95411

PARTS LIST

ORIG DATE	CHKD DATE	APPR DATE	TITLE	REV	DATE	EO. NO.	SHEET	
TB 08/21/84	GS/PQ 10/17/84	GB 10/18/84	CIRCUIT BOARD ASSEMBLY, FRONT PANEL	D	03-03-86	16437	1/2	PL26563

ITEM NO.	SIZE	IND NO.	DWG NO./PART NO.	CUST DWG	REV	EO. NO.	DESCRIPTION	QTY
			CONTROL DWG					
	A		PL26563		-	-	CIRCUIT BOARD ASSEMBLY, FRONT PANEL (PARTS LIST)	-
	D		SC2775A	*	ref	-	SIGNAL CONDITIONER SCHEMATIC DIAGRAM	-
	C	1	26563	*	C	16062	CIRCUIT BOARD ASSEMBLY, FRONT PANEL	-
1	C	2	26635		C	16062	CIRCUIT BOARD, FRONT PANEL	1
	-	3	AW26635		C	16062	ARTWORK, CIRCUIT BOARD, FRONT PANEL	1
2	B	2	25997-27		B	15976	RIBBON CABLE ASSEMBLY, 20 COND	1
3	B	2	26007-34		B	15976	RIBBON CABLE ASSEMBLY, 26 COND	1
4	-	2	EX50		-	-	ELEVATOR SOCKET, 20 PIN	2
5	A	2	26080		A	15436	SPACER	1
CR1	-	2	ECR290		-	-	DISPLAY, LED, MV57164	1
CR2	-	2	ECR290		-	-	DISPLAY, LED, MV57164	1
CR3	-	2	0208-11		-	-	DIODE, 1N916B	1
CR4	-	2	0208-11		-	-	DIODE, 1N916B	1
R1	-	2	0305-621		-	-	RESISTOR, 620 Ω	1
R2	-	2	0305-152		-	-	RESISTOR, 1.5K	1
R3	-	2	0305-122		-	-	RESISTOR, 1.2K	1

* DENOTES CUSTOMER DWG

ENDEVCO PARTS LIST

ITEM NO.	SIZE	IND NO.	DWG NO./PART NO.	CUST DWG	REV	EO NO.	DESCRIPTION	QTY
R4	-	2	ER3435		-	-	POTENTIOMETER, 50K	1
R5	-	2	0309-4021		-	-	RESISTOR, 4.02K, 1%	1
S1	-	2	ES264		-	-	SWITCH, ROTARY, 1 POLE, 10 POS	1
S2	-	2	ES266		-	-	SWITCH, ROTARY, 2 POLE, 4 POS	1
S3	-	2	ES266		-	-	SWITCH, ROTARY, 2 POLE, 4 POS	1
S4	-	2	ES271		-	-	SWITCH, TOGGLE, SPDT	1
S5			---				Not used on this assembly	
S6			---				Not used on this assembly	
S7	-	2	ES271		-	-	SWITCH, TOGGLE, SPDT	1
S8	-	2	ES271		-	-	SWITCH, TOGGLE, SPDT	1

IMPORTANT NOTICE: INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO CONFIDENTIAL. REPRODUCTION, DUPLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY.

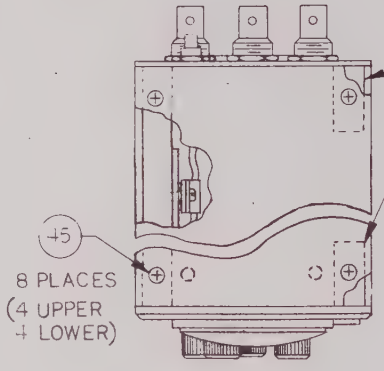

TOP VIEW



VIEW "C"
CABLE REMOVED
FOR CLARITY

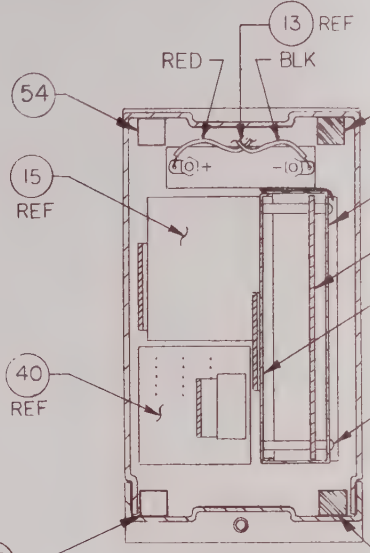

SECTION B-B

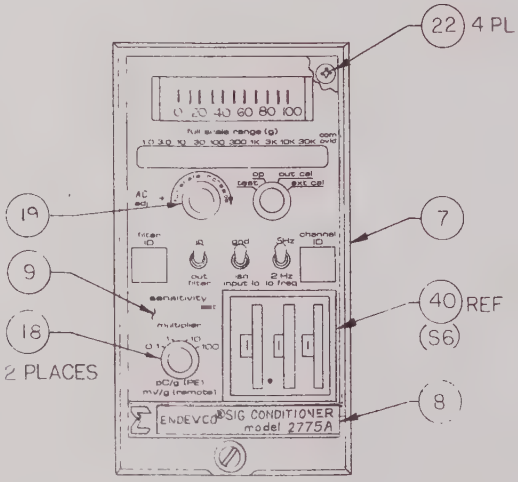

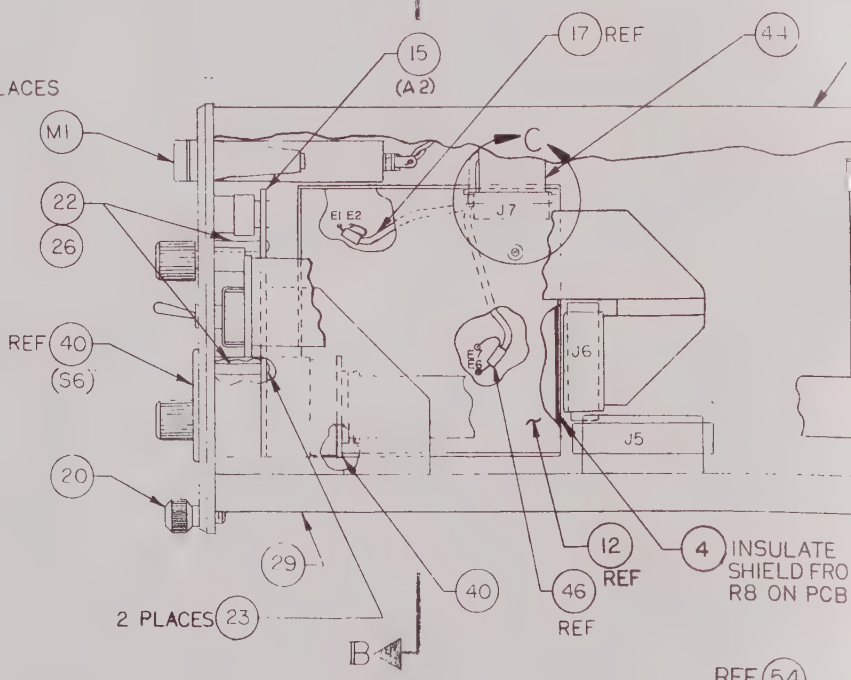



5. DELETED

4. VERIFY THAT S9 IS IN POSITION 2.

3. APPLY A DROP OF EHX97 (RTV118) OR EQUIVALENT AT END OF J10 TO INSURE PLUGS REMAIN INSERTED IN SOCKETS.

2. SOLDER PER REQUIREMENT 5 OF MIL-STD-454 USING Sn63 SOLDER PER QQ-S-571.

1. COMPLETED ASSEMBLY MUST MEET REQUIREMENTS OF PS2775A.

NOTES: UNLESS OTHERWISE SPECIFIED

NOTE: UNLESS OTHERWISE SPECIFIED
INTERPRET DIMENSIONING AND TOLERANCING PER ANSI-Y14.5
REMOVE ALL BURRS
COUNTERSINK INTERNAL THDS 90° TO MAJOR DIA
CHAM EXT THDS 45° TO MINOR DIA
ALL THD LENGTHS ARE FOR MIN FULL THDS
THDS PER MIL-S-7742
ALL DIM APPLY AFTER PLATING
63 ALL MACHINED SURFACES
CONCENTRICITY .005 FIR
BREAK SHARP EDGES .005 TO .010
MACHINED FILLET RADII .005 TO .015
WELD SYMBOLS PER AWS A2.0 (ANSI Y32.3)

DIETERICH POST CLEARPRINT

REVISIONS				
REV	E.O.	DESCRIPTION	DATE	APPROVED
A	15827	RELEASED	TB 10-3-84	GB 10/4/84
B	15976	RE-ROUTED RIBBONS TO J6 & J9 ADDED ITEM 42.	ET 11-30-84	GB 12/4/84
C	16062	ADDED ITEMS 46-49	TB 4-17-85	GB 5/6/85
D	16531	ADDED ITEMS 50, 51 & 52. ITEMS 21 & 25 WERE 6 PLACES	5/14/86	GB 5/20/86
E	17024	DELETED 34(EHW15) & 49(EHW69) AT ITEM 26.	DB 5/14/87	GB 5/11/87
F	17147	DELETED ITEMS 4,5,6. CHANGED ITEM 3 FROM MOUNTING BAR TO MOUNT, MOLDED. ADDED ITEM 4 AND NOTE 5.	DB 9-1-87	GB 9/25/87
G	17535	DELETED ITEMS 4 & 21. DELETED NOTE 5. ADDED ITEMS 53 & 54. ADDED VIEW "C". RELOCATED ITEM 31 CALLOUT.	ILR 12/19/88	GB 2/14/89
H	18807	REVISED ITEMS: 3, 53, 54 TO CONFORM WITH PL CHANGES. ADDED DETAIL C.	TD 7/9/90	GB 7/16/90
J	19451	DELETED ITEM 42. (Fuse Cover)	DB 6-28-91	GB 7/8/91
J1	19813	AT NOTE 3 DELETED "...J5, J6, J7, J8..."	DB 7-8-91	[illegible]
K	19924	DELETED ITEM 35 (TEFLON TAPE)	TB 2-18-92	GB 2/24/92
L	20107	ADDED ITEM 4	TB 5-27-92	GB 6/2/92

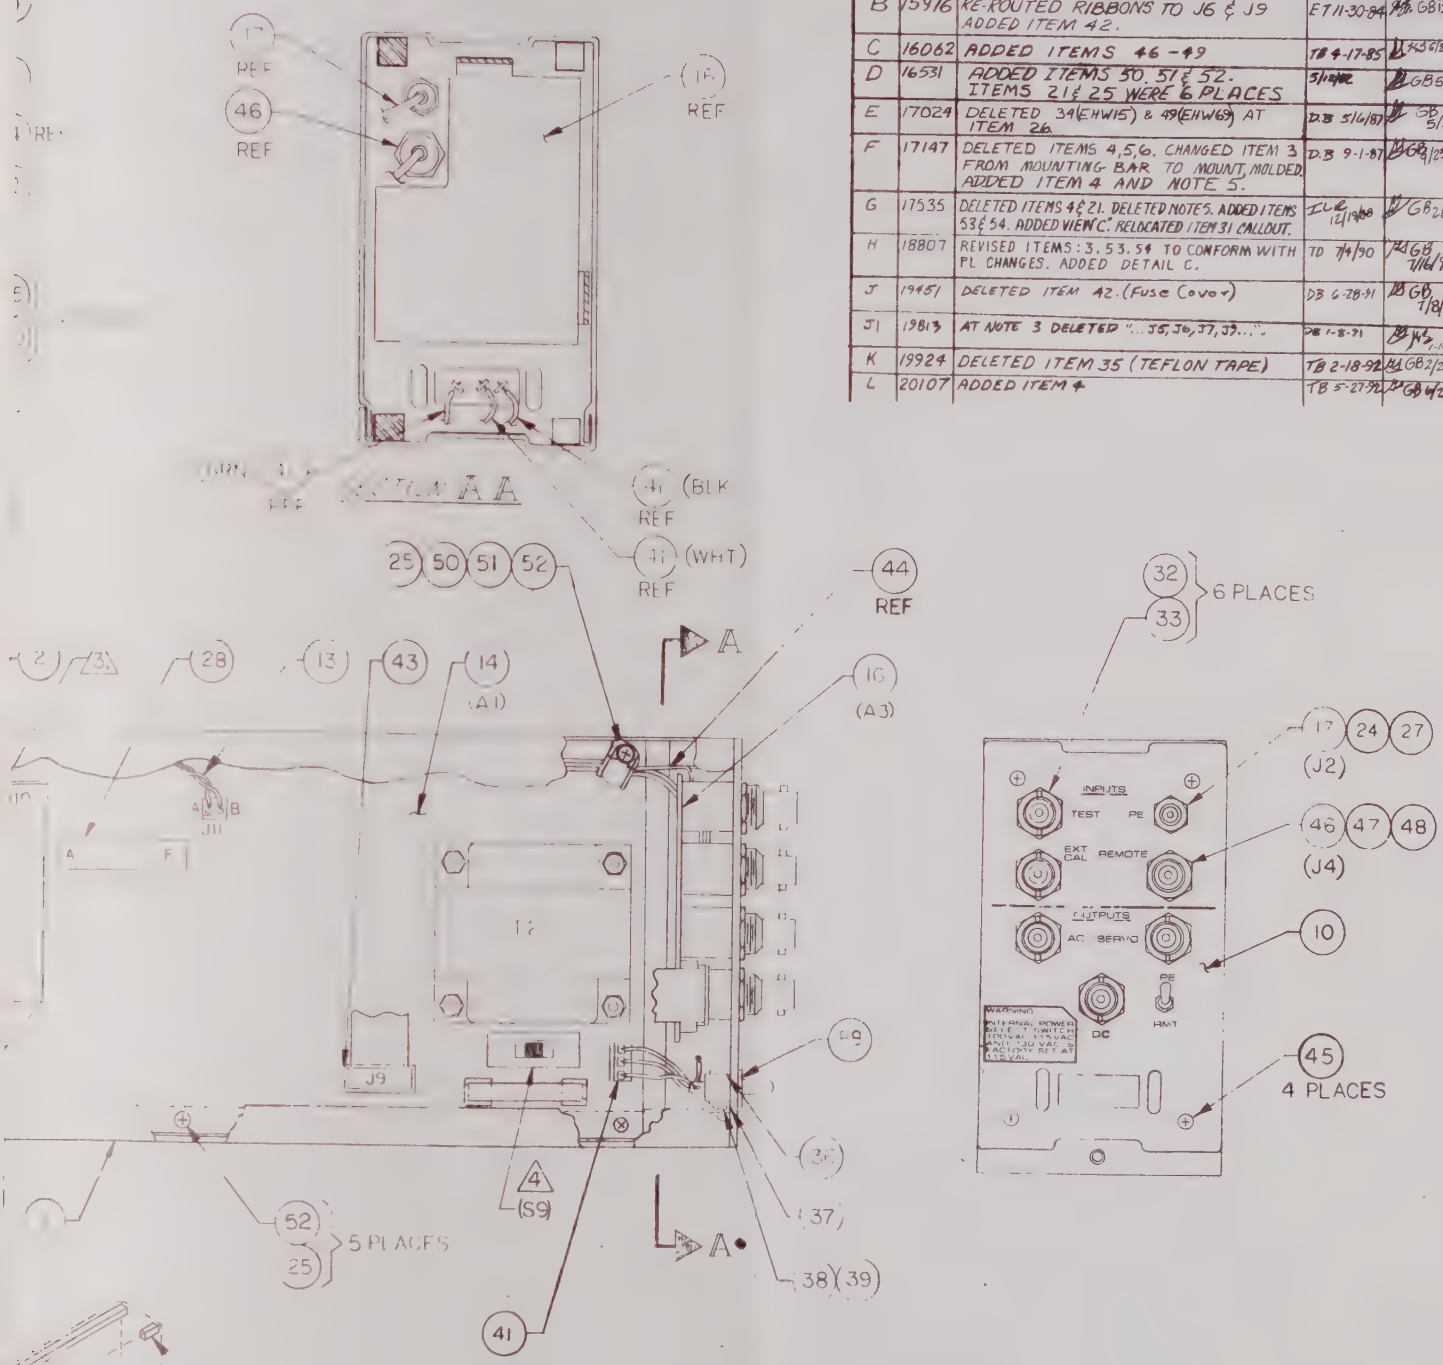

ITEM NO.	QTY REQD	CODE IDENT	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL	SPECIFICATION

PARTS LIST

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES. TOLERANCES ON: FRACTIONS ± DECIMALS .X ± .XX ± .XXX ± ANGLES ±

CONTRACT NO.

DR BY

CHK BY J. Swanson 10/17/84

APPROVED BY G. Bullard 10/18/84

MATERIAL SEE PL9775A

FINISH

DO NOT SCALE DRAWING

ENDEVCO SAN JUAN CAPISTRANO, CA 92675

SIGNAL CONDITIONER FINAL ASSEMBLY

SIZE	CODE IDENT NO.	DWG NO.	REV
D	95411	92775A	L

SCALE

SHEET OF

DRILL DIA.	TOL
.0135 THRU .125	+ .004 .001
.126 THRU .250	+ .005 .001
.251 THRU .500	+ .006 .001
.501 THRU .750	+ .008 .001
.751 THRU 1.000	+ .010 .001
1.001 THRU 2.000	+ .012 .001

NEXT ASSY	USED ON
	92775A

APPLICATION

NONE

92775A

IMPORTANT NOTICE: INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO PRIVATE. REPRODUCTION, DUPLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY.

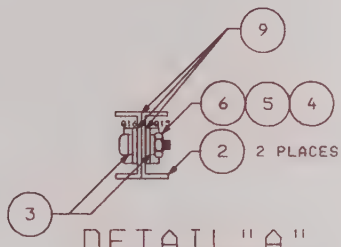

DETAIL "A"

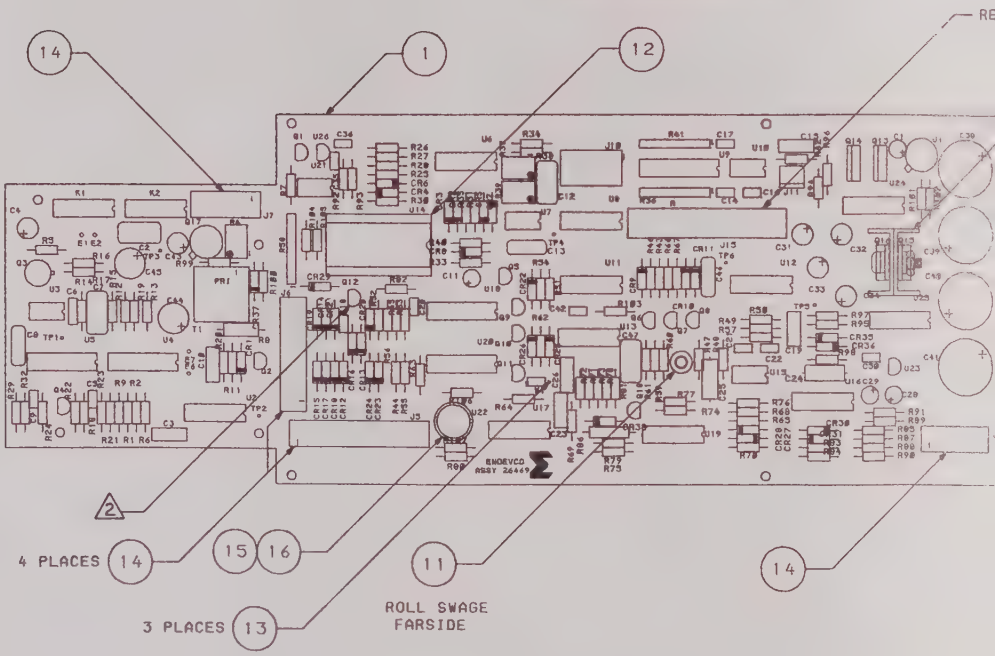

2 FOR -3 ASSY ONLY, ADD JUMPER BETWEEN C & E OF Q12.

1. SOLDER USING Sn63 SOLDER PER QQ-S-571.

NOTES: UNLESS OTHERWISE SPECIFIED

REVISIONS					
REV	EO	DESCRIPTION	BY/DATE	CHK	APPR
G	18248	REDRAWN, ADDED ITEMS 3 & 9, (INSULATION AT Q15 & Q16)	TB 8-22-89	GS 8 29-9	GB 8 29-9
H	18357	ADDED ITEMS 15 & 16; ADDED C47, C48, R106 & R107	ILR 11-3-89		GB 11/3/89
J	18898	ADDED NOTE 2.	DB 8-24-90		GB 9/24/90

8 DISCARD METAL CLIPS.

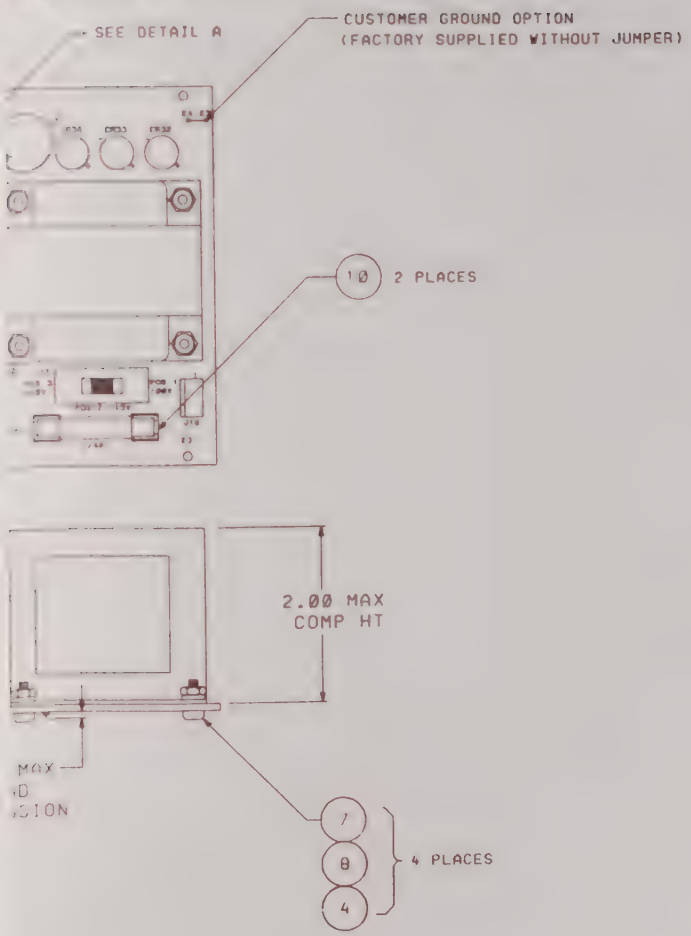

ITEM NO	PART NO	DESCRIPTION	QTY REQD

PARTS LIST

UNLESS OTHERWISE SPECIFIED
INTERPRET DIM & TOL PER ANSI Y14.5M – 1982
DO NOT SCALE DRAWING
REMOVE BURRS
COUNTERSINK INTERNAL THDS 90° TO MAJOR DIA
CHAM EXT THDS 45° TO MINOR DIA
THD LENGTHS AND DEPTHS ARE FOR MIN FULL THDS.
THDS PER MIL S-7742
DIMENSIONS APPLY AFTER FINISHING
63 √ ALL MACHINED SURFACES
TOTAL RUNOUT WITHIN .005
BREAK SHARP EDGES
.005 TO .010
MACHINED FILLET RADII .005 TO .015
WELDING SYMBOLS PER AWS A2.4
ABBREVIATIONS PER MIL-STD-12

92775A	92775A
NEXT ASSY	USED ON
APPLICATIONS	

UNLESS OTHERWISE SPECIFIED:
DIMENSIONS ARE IN INCHES.
TOLERANCES ON:
FRACTIONS ± / DECIMALS .X ± .XX ± .XXX ± ANGLES ± /

MATERIAL: SEE PL26469

FINISH:

CONTRACT NUMBER:

CONTRACTOR:

DRAWN BY/DATE: T.BARNES 10-18-84

CHECKER/DATE: G.S./P.Q. 10-18-84

APPROVAL/DATE: BRISENO 10-18-84

APPROVAL/DATE:

ENDEVCO SAN JUAN CAPISTRANO, CA 92675

SIGNAL CONDITIONER CIRCUIT BOARD ASSY (A1)

SIZE	FSCM	DWG NO.	REV
D	95411	26469	J

SCALE 1/1 | CAD C93.BRD | SHEET 1 OF 1

IMPORTANT NOTICE INFORMA... CONFIDENTIAL REPRODUCTI... GRANTED BY WRITTEN PERMISS... ...LOSED BY THIS DRAWING IS ENDEVCO ...CATION, OR MANUFACTURING RIGHTS ...Y

REVISIONS					
REV	EO	DESCRIPTION	DATE	CHK	APPR
A	15827	RELEASED	TB 10-3-84		
B	16062	REVISED CKTY, REMOVED J4	TB 9-17-85		

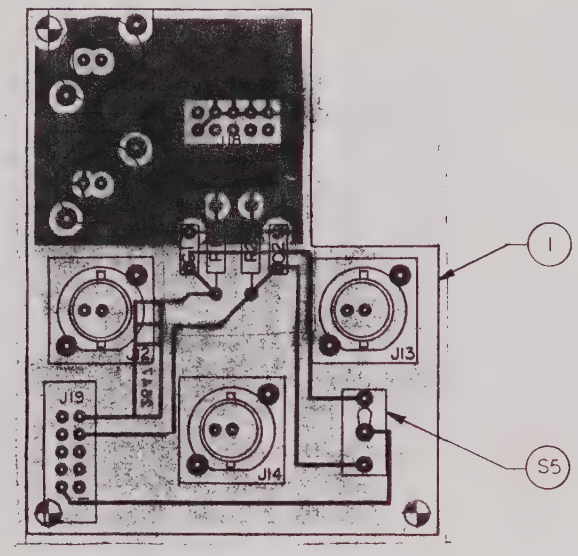

1. SOLDER PER REQUIREMENT 5 OF MIL-STD-454 USING Sn63 SOLDER PER QQ-S-571.

NOTES: UNLESS OTHERWISE SPECIFIED

UNLESS OTHERWISE SPECIFIED:
INTERPRET DIM & TOL PER ANSI Y14.5
REMOVE BURRS
COUNTERSINK INTERNAL THDS 90° TO MAJOR DIA
CHAM EXT THDS 45° TO MINOR DIA
THD LENGTHS ARE FOR MIN FULL THDS
THDS PER MIL-S-7742
DIMENSIONS APPLY AFTER FINISHING
63√ MACHINED SURFACES
CONCENTRICITY .005 Ø RFS
BREAK SHARP EDGES .005 TO .010
MACHINED FILLET RADII .005 TO .015
WELDING SYMBOLS PER AWS A2 4
ABBREVIATIONS PER MIL-STD-12

HOLE DIA	TOL
.0135 THRU .125	+.004/-.001
.126 THRU .250	+.005/-.001
.251 THRU .500	+.006/-.001
.501 THRU .750	+.008/-.001
.751 THRU 1.000	+.010/-.001
1.001 THRU 2.000	+.012/-.001

92775A	2775A
NEXT ASSY	USED ON
APPLICATIONS	

ITEM NO	QTY REQD	FSCM	PART OR IDENTIFYING NO	NOMENCLATURE OR DESCRIPTION	MATERIAL	SPECIFICATION

PARTS LIST

UNLESS OTHERWISE SPECIFIED:
DIMENSIONS ARE IN INCHES.
TOLERANCES ON:
FRACTIONS ± / | DECIMALS .X ± / .XX ± / .XXX ± / | ANGLES ± /

MATERIAL: SEE PL26476

FINISH

DO NOT SCALE DRAWING

CONTRACT

DWN/DATE: T. BARNES 7-24-84
CHK/DATE: [illegible] 10-17-84

APPROVED BY
NAME/DATE: G Briseno 10/18/84
NAME/DATE:

ENDEVCO SAN JUAN CAPISTRANO, CA 92675
DIVISION OF BECTON, DICKINSON AND COMPANY B-D

CIRCUIT BOARD ASSEMBLY REAR PANEL

SIZE	FSCM	DWG NO	REV
C	95411	26476	B

SCALE 2/1 SHEET OF

26476 B

IMPORTANT NOTICE. INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO CONFIDENTIAL. REPRODUCTION, PUBLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY

REVISIONS					
REV	EO	DESCRIPTION	DATE	CHK	APPR
A	15827	RELEASED	TB 10-8-84		
B	15976	CORRECTED PICTURE TO SHOW E6, E7, E8 PADS	TB 12-10-84		
C	16062	REVISED CKTRY	TB 5-29-85		

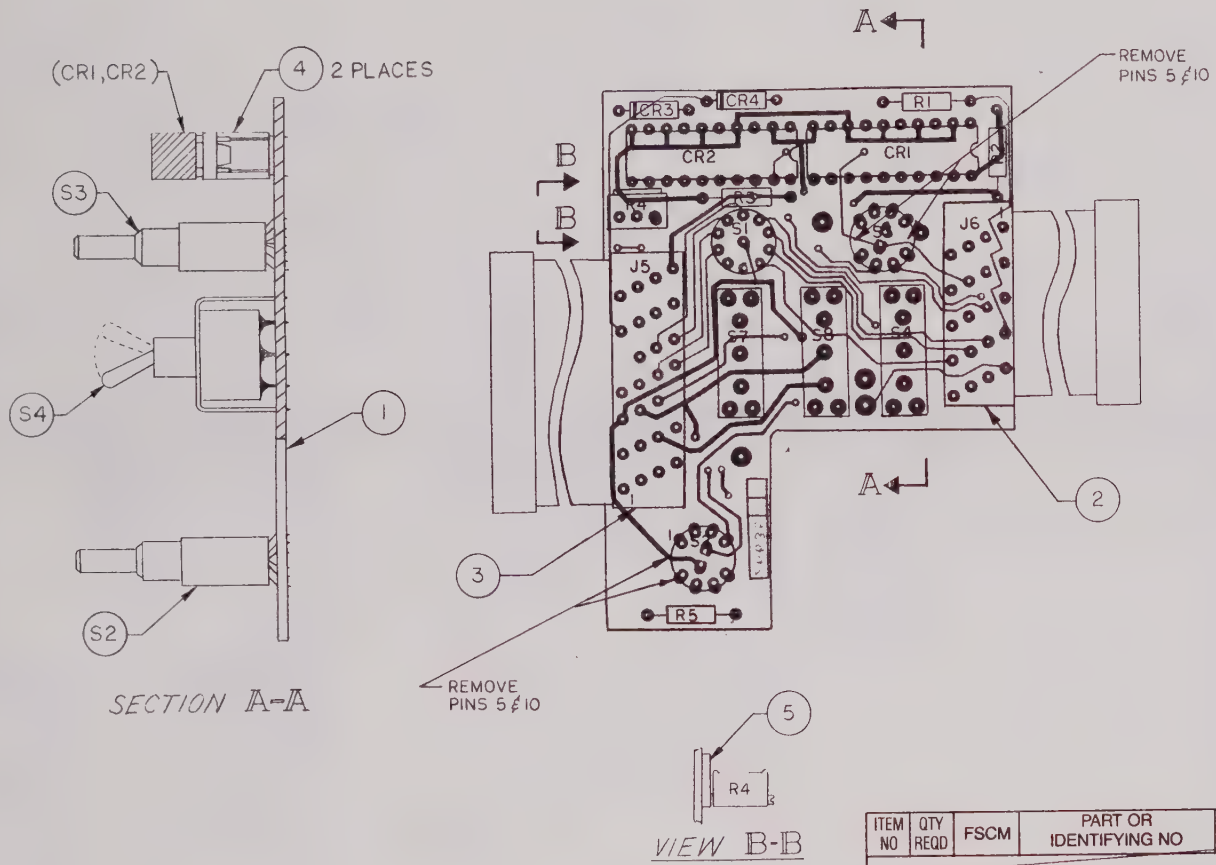

1. SOLDER PER REQUIREMENT 5 OF MIL-STD-454 USING Sn63 PER QQ-S-571.

NOTES: UNLESS OTHERWISE SPECIFIED

UNLESS OTHERWISE SPECIFIED:
INTERPRET DIM & TOL PER ANSI Y14.5
REMOVE BURRS
COUNTERSINK INTERNAL THDS 90° TO MAJOR DIA
CHAM EXT THDS 45° TO MINOR DIA
THD LENGTHS ARE FOR MIN FULL THDS
THDS PER MIL-S-7742
DIMENSIONS APPLY AFTER FINISHING
63√ MACHINED SURFACES
CONCENTRICITY .005 Ø RFS
BREAK SHARP EDGES .005 TO .010
MACHINED FILLET RADII .005 TO .015
WELDING SYMBOLS PER AWS A2.4
ABBREVIATIONS PER MIL-STD-12

HOLE DIA	TOL
.0135 THRU .125	+.004/-.001
.126 THRU .250	+.005/-.001
.251 THRU .500	+.006/-.001
.501 THRU .750	+.008/-.001
.751 THRU 1.000	+.010/-.001
1.001 THRU 2.000	+.012/-.001

NEXT ASSY	USED ON
92775A	2775A

APPLICATIONS

ITEM NO	QTY REQD	FSCM	PART OR IDENTIFYING NO	NOMENCLATURE OR DESCRIPTION	MATERIAL	SPECIFICATION

PARTS LIST

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES. TOLERANCES ON: FRACTIONS ± / DECIMALS .X ± .XX ± .XXX ± ANGLES ±

CONTRACT

DWN/DATE T. BARNES 8-21-84
CHK/DATE Robinson 10/16/84

MATERIAL
SEE PL26563

APPROVED BY
NAME/DATE G Briseno 10/16/84
NAME/DATE

FINISH

DO NOT SCALE DRAWING

ENDEVCO SAN JUAN CAPISTRANO, CA 92675
DIVISION OF BECTON, DICKINSON AND COMPANY B-D

CIRCUIT BOARD ASSEMBLY, FRONT PANEL

SIZE	FSCM	DWG NO	REV
C	95411	26563	C

SCALE 2/1 SHEET 1 OF 1

26563

IMPORTANT NOTICE INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO CONFIDENTIAL. REPRODUCTION, DUPLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY

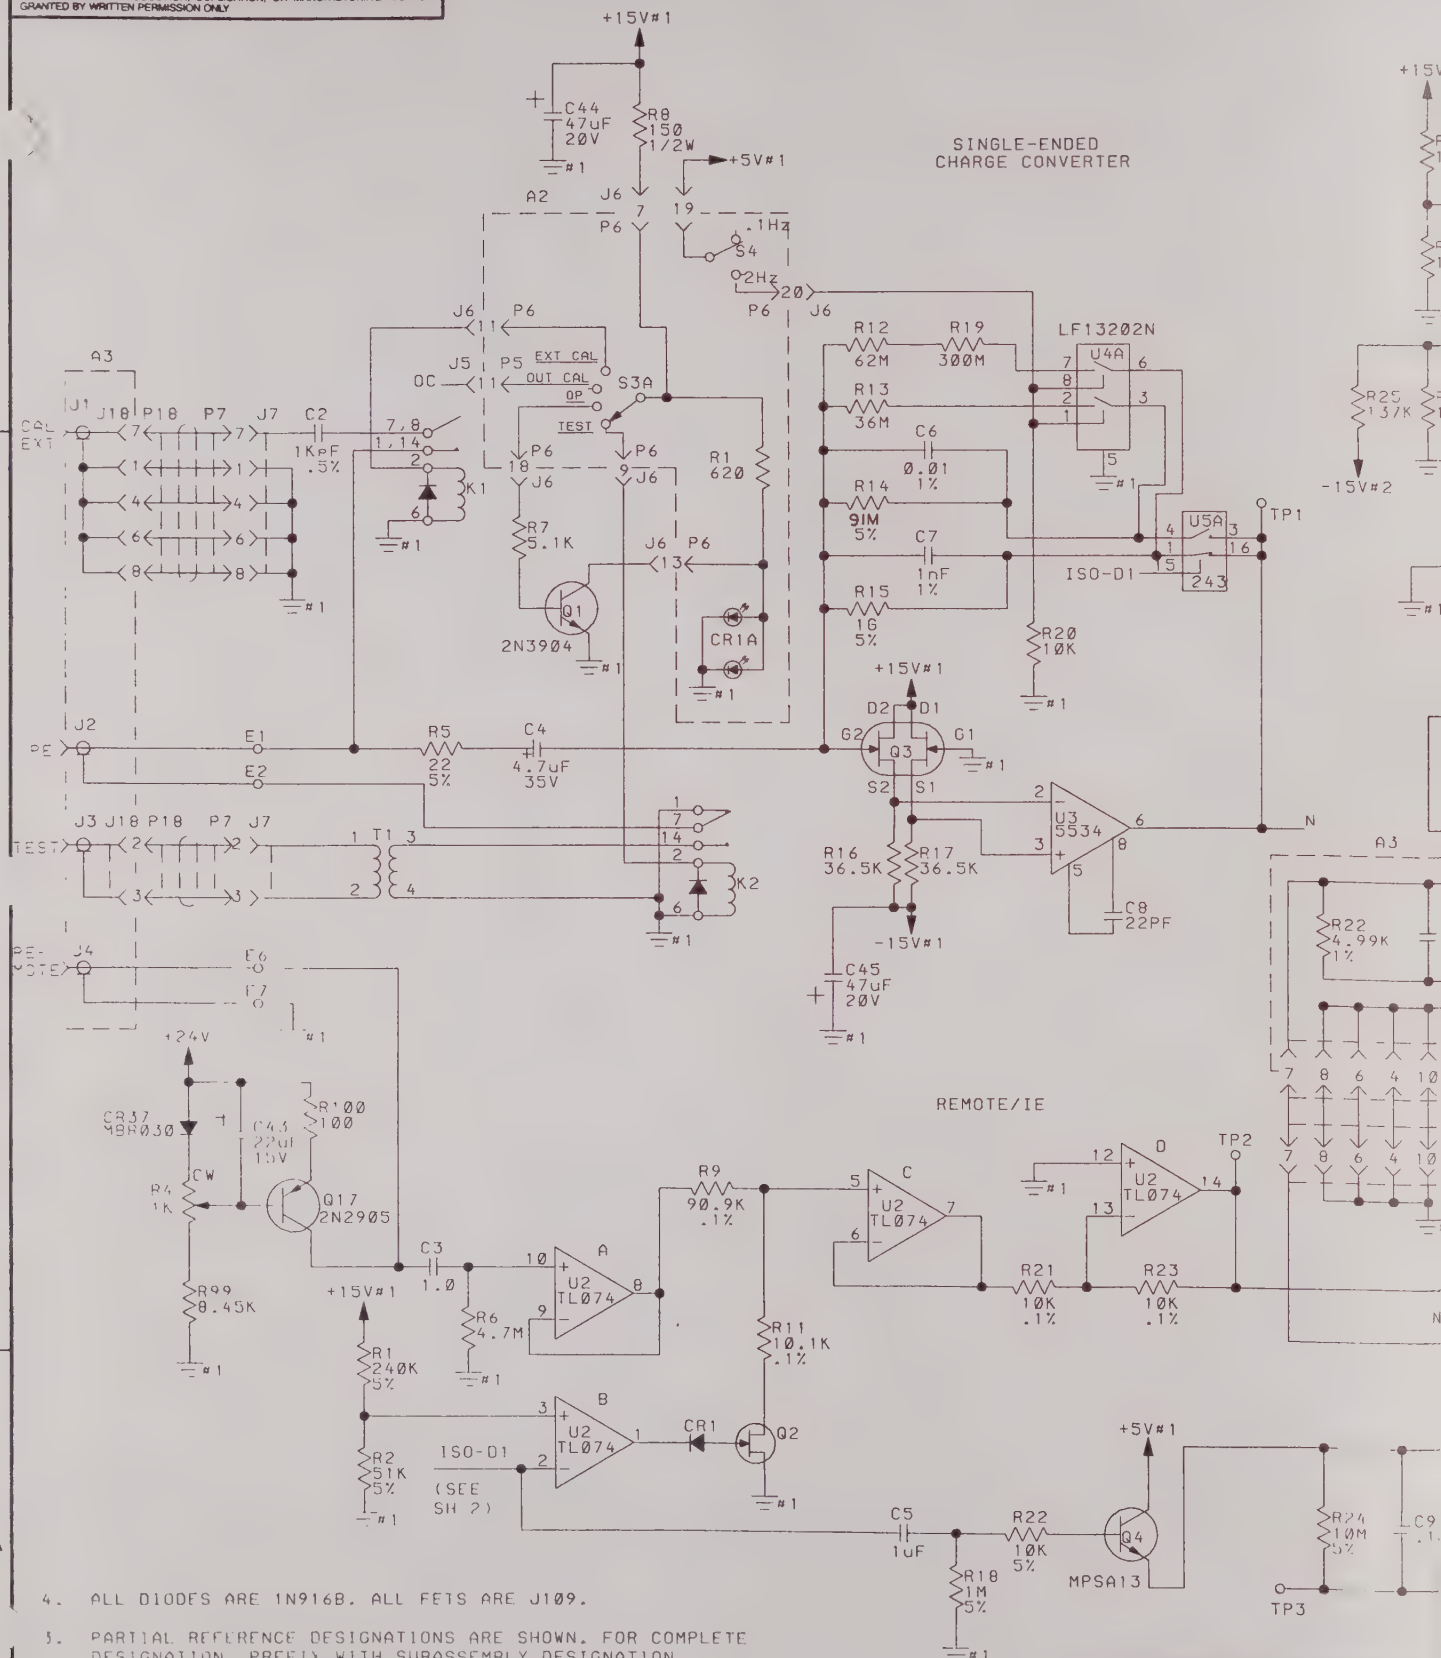

4. ALL DIODES ARE 1N916B. ALL FETS ARE J109.

5. PARTIAL REFERENCE DESIGNATIONS ARE SHOWN. FOR COMPLETE DESIGNATION. PREFIX WITH SUBASSEMBLY DESIGNATION.

2. ALL CAPACITOR VALUES ARE IN MICROFARADS.

1. ALL RESISTOR VALUES ARE IN OHMS, 1%, 1/10W, .1% ARE 1/10W & 5% ARE 1/4W.

NOTES: UNLESS OTHERWISE SPECIFIED

UNLESS OTHERWISE SPECIFIED
INTERPRET DIM & TOL PER ANSI Y14.5
REMOVE BURRS
COUNTERSINK INTERNAL THDS 90° TO MAJOR DIA
CHAM EXT THDS 45° TO MINOR DIA
THD LENGTHS ARE FOR MIN FULL THDS
THDS PER MIL-S-7742
DIMENSIONS APPLY AFTER FINISHING
63√ MACHINED SURFACES
CONCENTRICITY .005 Ø RFS
BREAK SHARP EDGES .005 TO .010
MACHINED FILLET RADII .005 TO .015
WELDING SYMBOLS PER AWS A2.4
ABBREVIATIONS PER MIL-STD-12

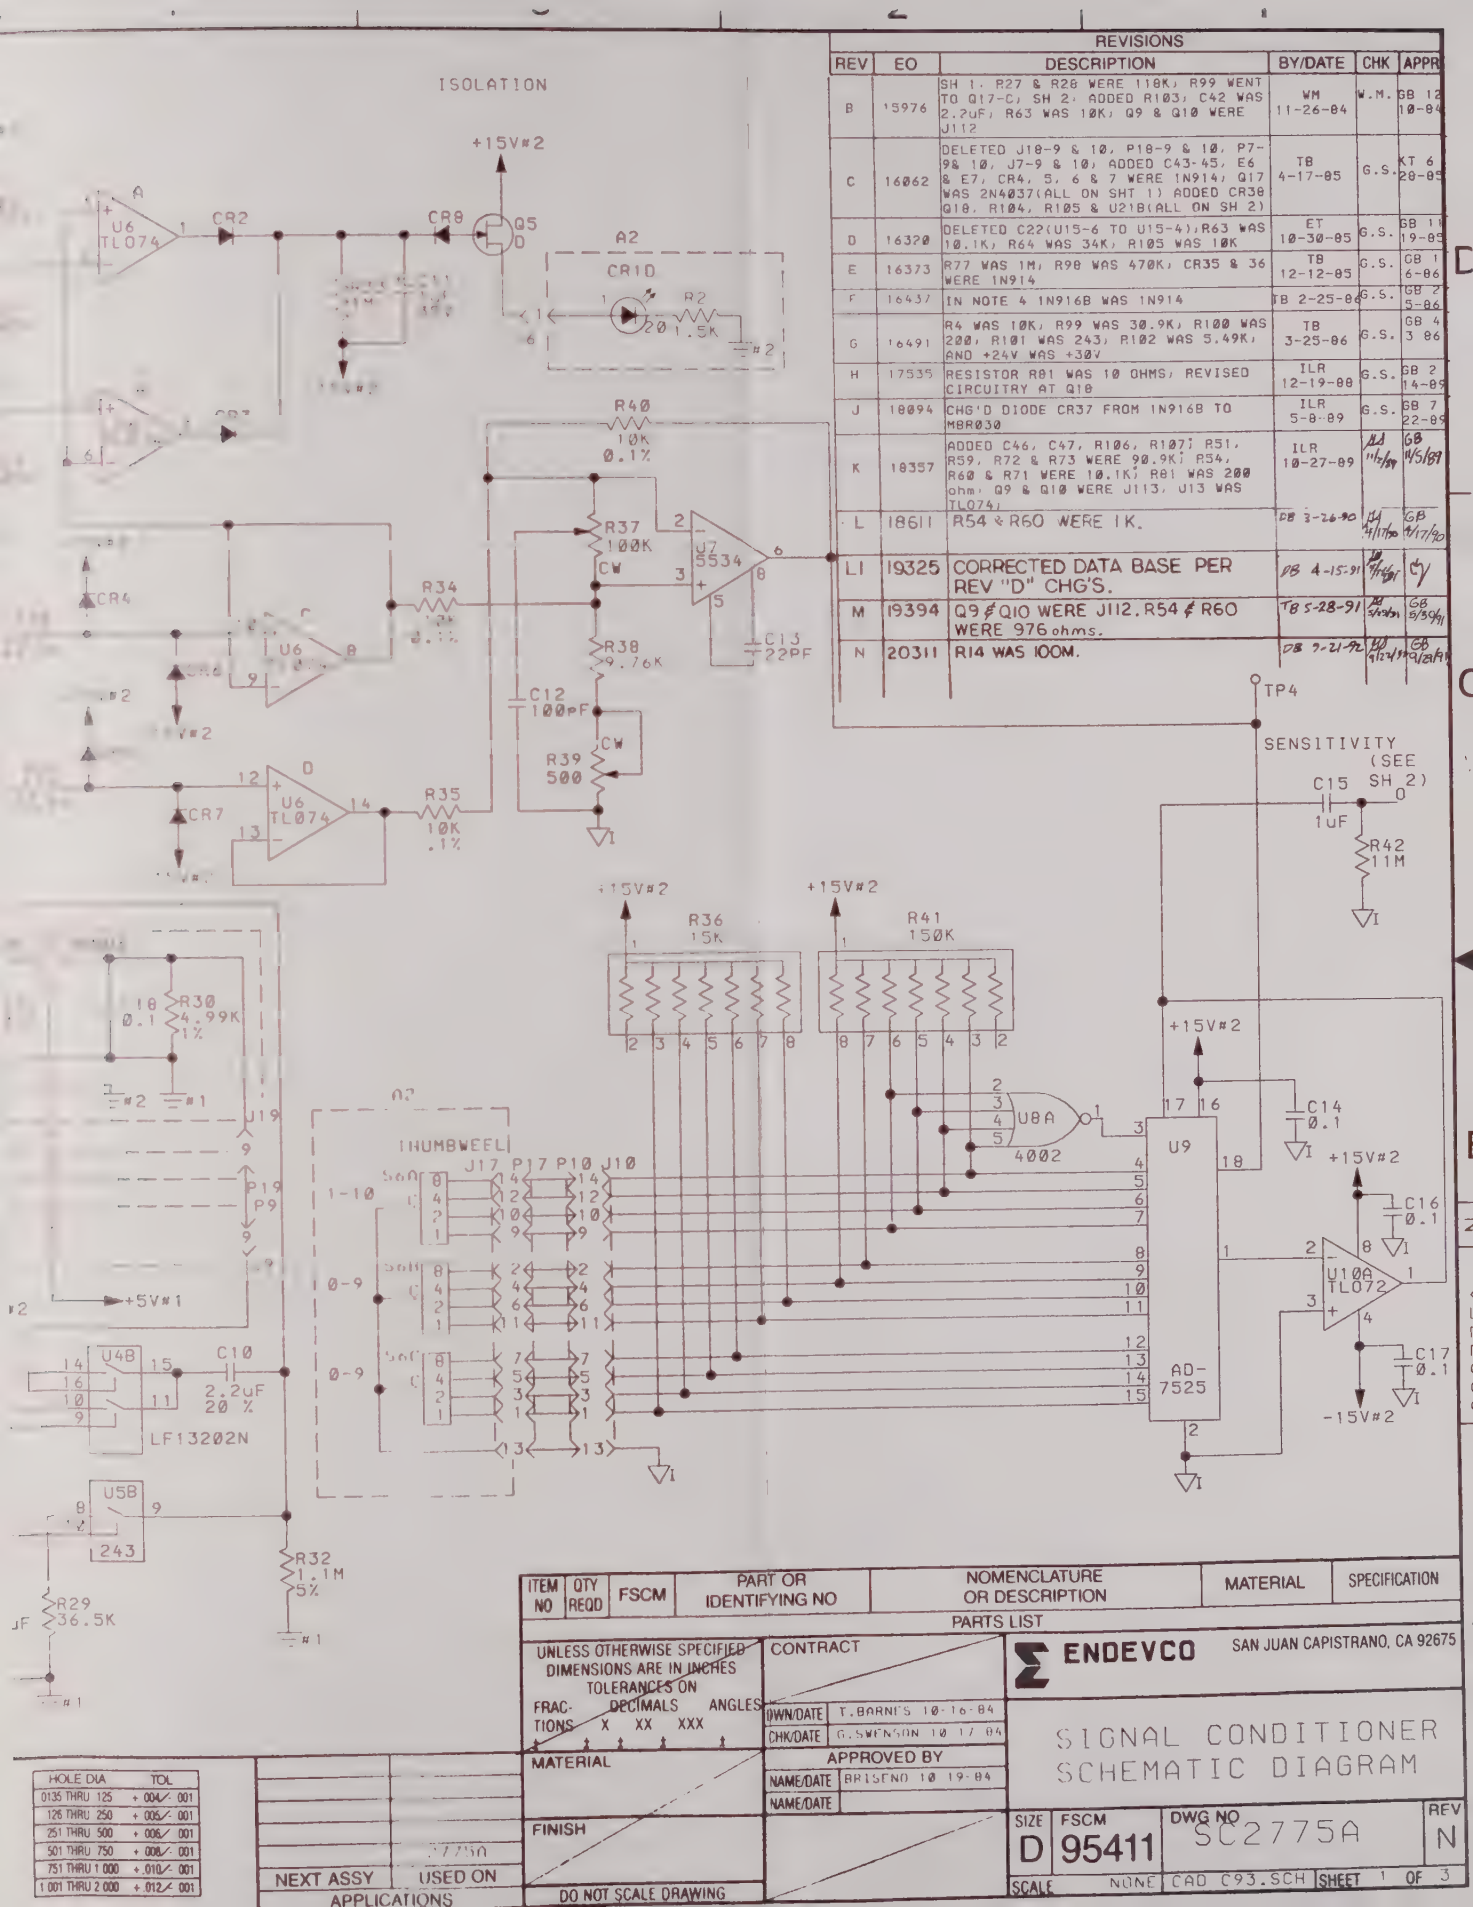

REVISIONS					
REV	EO	DESCRIPTION	BY/DATE	CHK	APPR
B	15976	SH 1, R27 & R28 WERE 110K; R99 WENT TO Q17-C; SH 2, ADDED R103, C42 WAS 2.2uF; R63 WAS 10K; Q9 & Q10 WERE J112	WM 11-26-84	W.M.	GB 12 10-84
C	16062	DELETED J10-9 & 10, P10-9 & 10, P7-9& 10, J7-9 & 10; ADDED C43-45, E6 & E7, CR4, 5, 6 & 7 WERE 1N914; Q17 WAS 2N4037(ALL ON SHT 1) ADDED CR38 Q18, R104, R105 & U21B(ALL ON SH 2)	TB 4-17-85	G.S.	KT 6 28-85
D	16320	DELETED C22(U15-6 TO U15-4);R63 WAS 10.1K; R64 WAS 34K; R105 WAS 10K	ET 10-30-85	G.S.	GB 11 19-85
E	16373	R77 WAS 1M; R98 WAS 470K; CR35 & 36 WERE 1N914	TB 12-12-85	G.S.	GB 1 6-86
F	16437	IN NOTE 4 1N916B WAS 1N914	TB 2-25-86	G.S.	GB 2 5-86
G	16491	R4 WAS 10K; R99 WAS 30.9K; R100 WAS 200; R101 WAS 243; R102 WAS 5.49K; AND +24V WAS +30V	TB 3-25-86	G.S.	GB 4 3 86
H	17535	RESISTOR R81 WAS 10 OHMS; REVISED CIRCUITRY AT Q18	ILR 12-19-88	G.S.	GB 2 14-89
J	18094	CHG'D DIODE CR37 FROM 1N916B TO MBR030	ILR 5-8-89	G.S.	GB 7 22-89
K	18357	ADDED C46, C47, R106, R107, R51, R59, R72 & R73 WERE 90.9K; R54, R60 & R71 WERE 10.1K; R81 WAS 200 ohm; Q9 & Q10 WERE J113, U13 WAS TL074;	ILR 10-27-89		GB 11/5/89
L	18611	R54 & R60 WERE 1K.	DB 3-26-90		GB 4/17/90
LI	19325	CORRECTED DATA BASE PER REV "D" CHG'S.	DB 4-15-91		
M	19394	Q9 & Q10 WERE J112. R54 & R60 WERE 976 ohms.	TB 5-28-91		GB 5/30/91
N	20311	R14 WAS 100M.	DB 7-21-92		GB 9/28/92

ITEM NO	QTY REQD	FSCM	PART OR IDENTIFYING NO	NOMENCLATURE OR DESCRIPTION	MATERIAL	SPECIFICATION

PARTS LIST

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ON
FRACTIONS X DECIMALS XX ANGLES XXX

CONTRACT

DWN/DATE T.BARNES 10-16-84
CHK/DATE G.SWENSON 10 17 84

APPROVED BY
NAME/DATE BRISENO 10 19-84
NAME/DATE

MATERIAL

FINISH

DO NOT SCALE DRAWING

ENDEVCO SAN JUAN CAPISTRANO, CA 92675

SIGNAL CONDITIONER
SCHEMATIC DIAGRAM

SIZE	FSCM	DWG NO	REV
D	95411	SC2775A	N

SCALE NONE CAD C93.SCH SHEET 1 OF 3

HOLE DIA	TOL
0135 THRU 125	+ 004 / - 001
126 THRU 250	+ 005 / - 001
251 THRU 500	+ 006 / - 001
501 THRU 750	+ 008 / - 001
751 THRU 1 000	+ 010 / - 001
1 001 THRU 2 000	+ 012 / - 001

NEXT ASSY | USED ON
APPLICATIONS

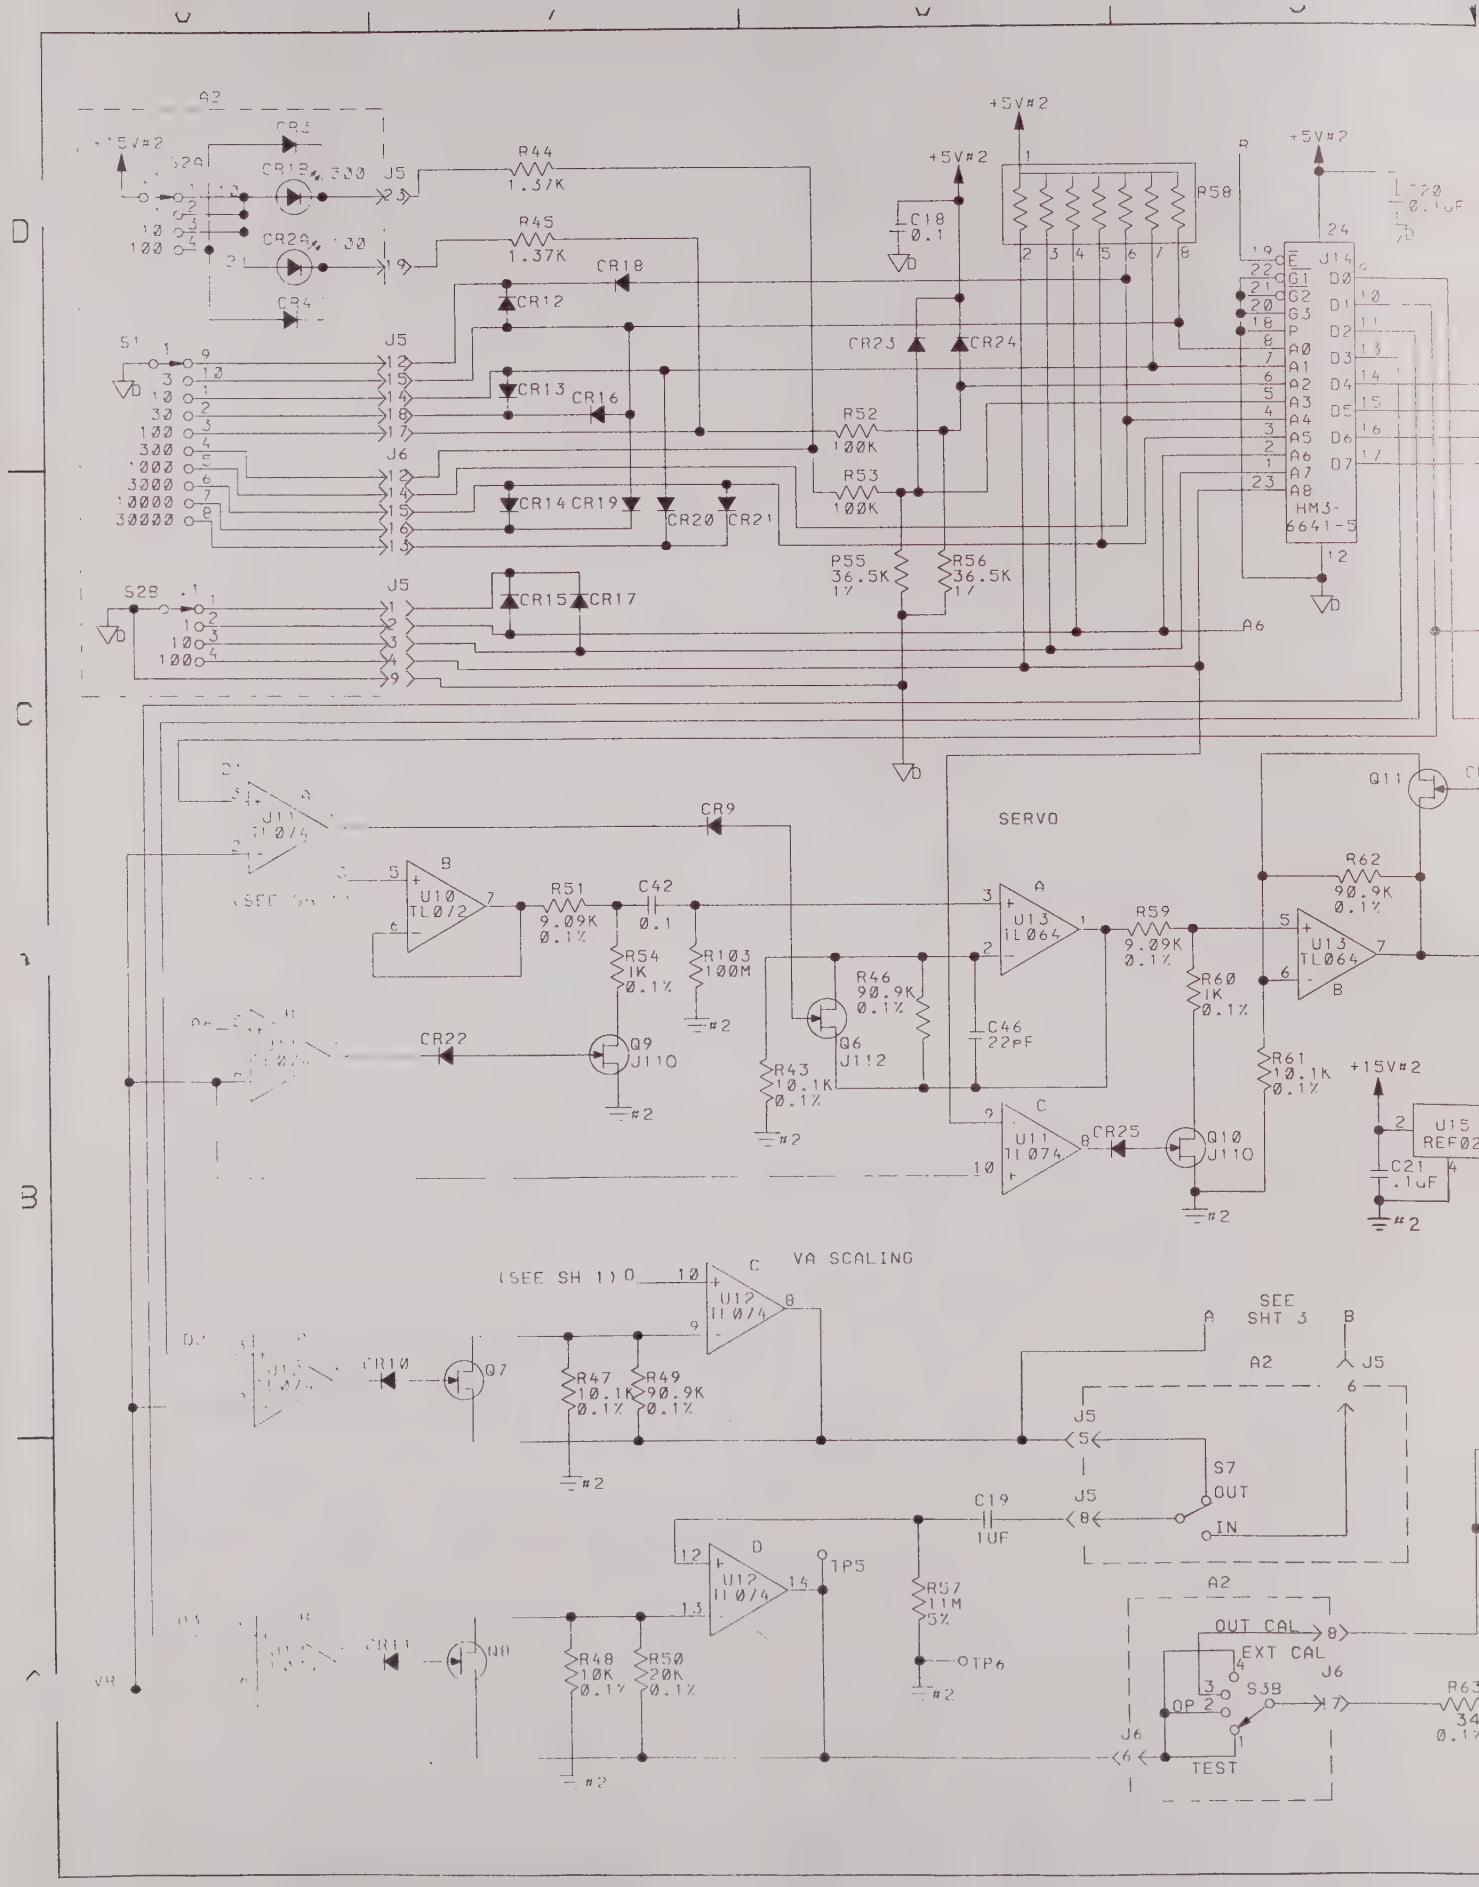
A2
+5V#2
CR13
CR22
CR3
CR4
S2A
S2B
S1
J5
J6
R44
1.37K
R45
1.37K
CR18
CR12
CR13
CR16
CR14
CR19
CR20
CR21
CR15
CR17
CR23
CR24
R52
100K
R53
100K
P55
36.5K
1%
R56
36.5K
1%
R58
C18
0.1
C20
0.1UF
J14
HM3-
6641-5
A6
SERVO
U11
TL074
U10
TL072
U13
TL064
R51
9.09K
0.1%
C42
0.1
R54
1K
0.1%
R103
100M
#2
CR9
CR22
Q9
J110
R46
90.9K
0.1%
Q6
J112
R43
10.1K
0.1%
C46
22pF
R59
9.09K
0.1%
R62
90.9K
0.1%
R60
1K
0.1%
R61
10.1K
0.1%
Q11
CR25
Q10
J110
+15V#2
U15
REF02
C21
.1uF
VA SCALING
(SEE SH 1) D
U12
TL074
CR10
Q7
R47
10.1K
0.1%
R49
90.9K
0.1%
SEE
SHT 3
A
B
J5
S7
OUT
IN
C19
1UF
TP5
R57
11M
5%
TP6
CR11
Q8
R48
10K
0.1%
R50
20K
0.1%
OUT CAL
EXT CAL
OP 2
S3B
TEST
J6
R63
34
0.1%

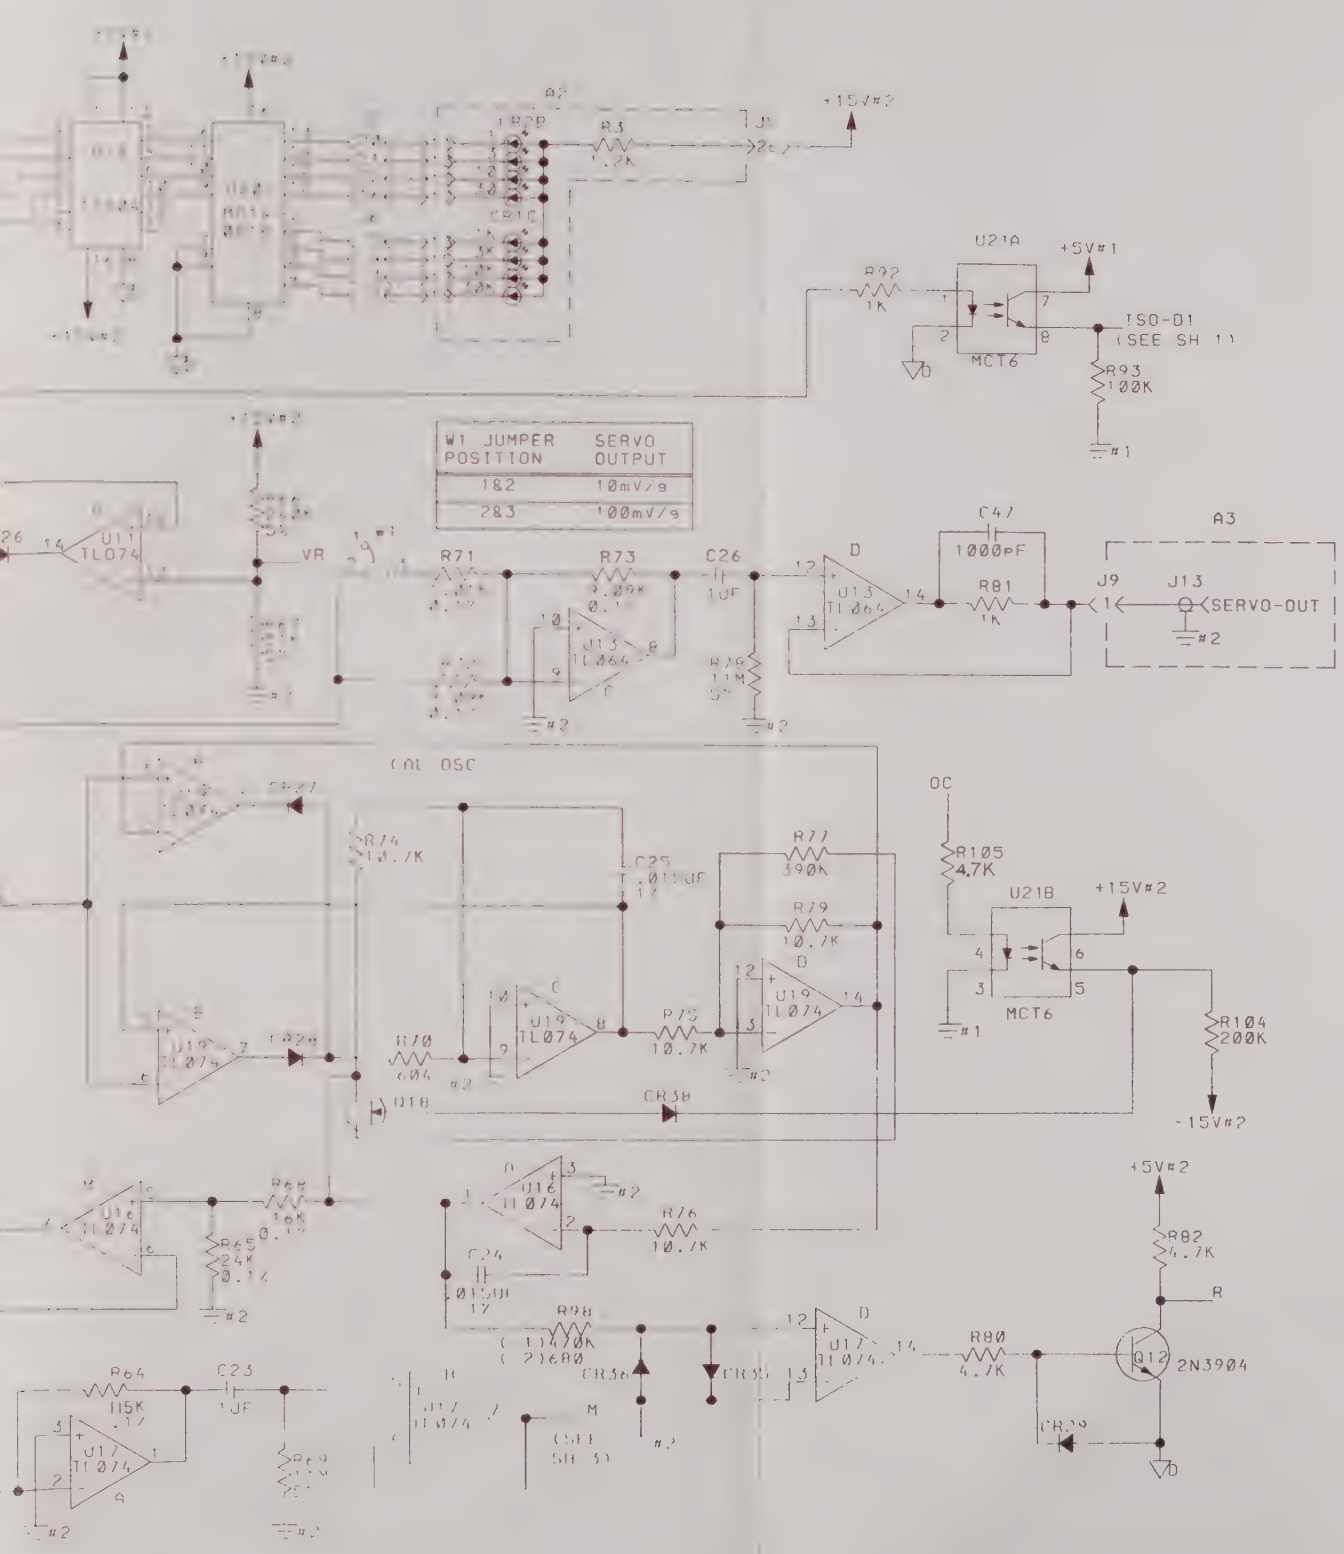

SIZE	FSCM	DWG NO	REV
D	95411	SC2775A	
SCALE		SHEET 2 OF 3	

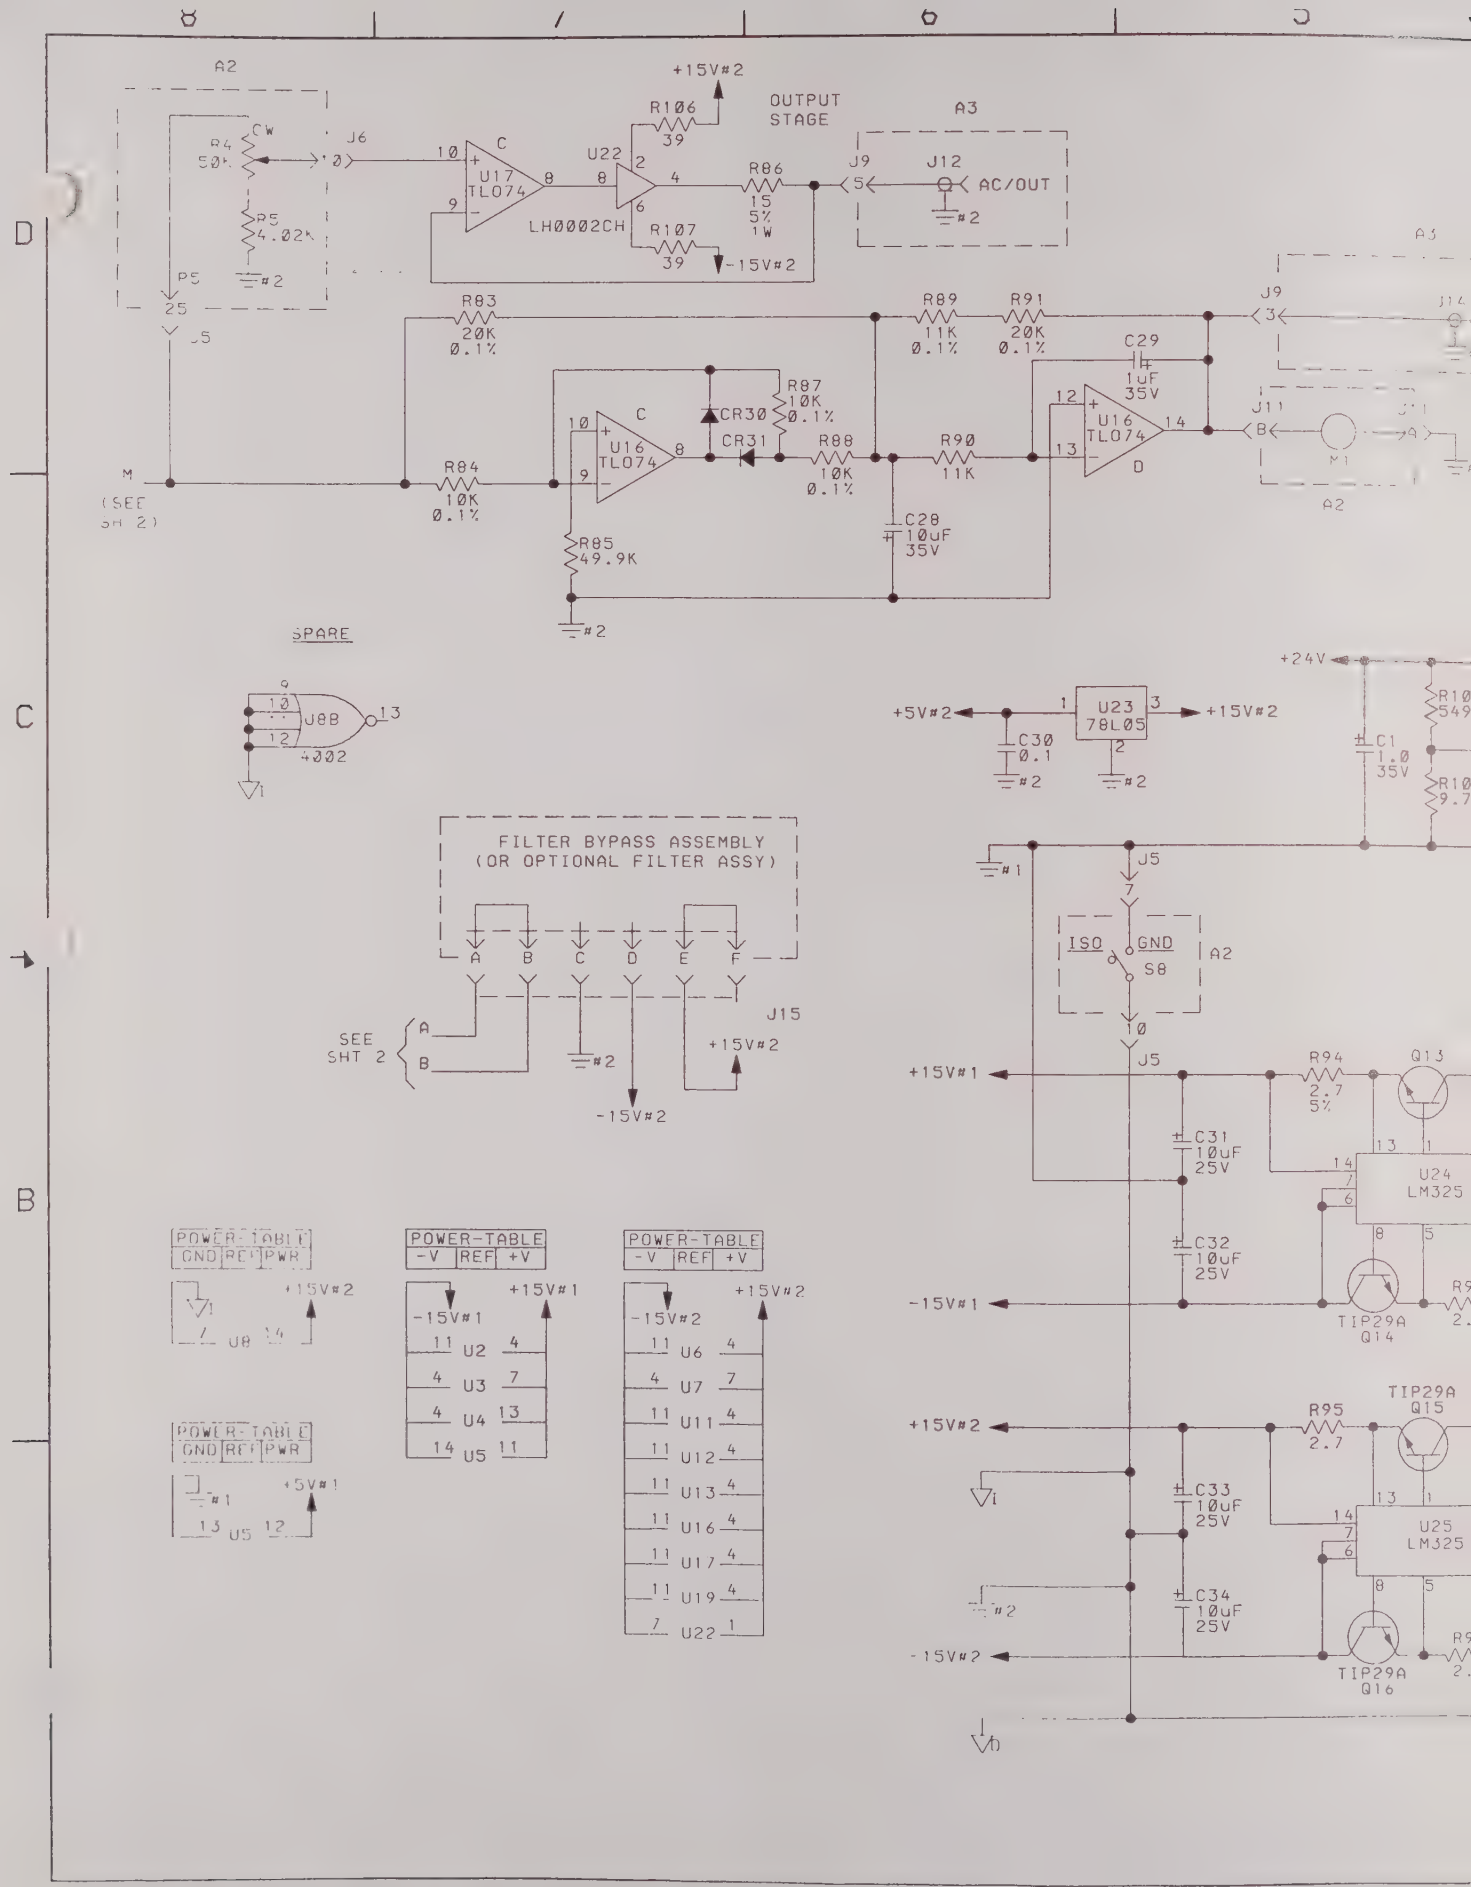
A2
R4 50K CW
R5 4.02K
P5
J6
U17 TL074
LH0002CH
U22
+15V#2
R106 39
R107 39
-15V#2
OUTPUT STAGE
A3
J9
J12
AC/OUT
R86 15 5% 1W
R83 20K 0.1%
R84 10K 0.1%
R85 49.9K
R87 10K 0.1%
R88 10K 0.1%
R89 11K 0.1%
R90 11K
R91 20K 0.1%
C28 10uF 35V
C29 1uF 35V
CR30
CR31
U16 TL074
J5
J11
M1
(SEE SH 2)
SPARE
U8B 4002
FILTER BYPASS ASSEMBLY (OR OPTIONAL FILTER ASSY)
A B C D E F
J15
SEE SHT 2
+24V
U23 78L05
C30 0.1
C1 1.0 35V
R10 549
R10 9.7
ISO GND S8
C31 10uF 25V
C32 10uF 25V
C33 10uF 25V
C34 10uF 25V
R94 2.7 5%
R95 2.7
Q13
Q14
Q15
Q16
U24 LM325
U25 LM325
TIP29A
POWER-TABLE
GND REF PWR
-V REF +V
U2
U3
U4
U5
U6
U7
U11
U12
U13
U16
U17
U19
U22
U8

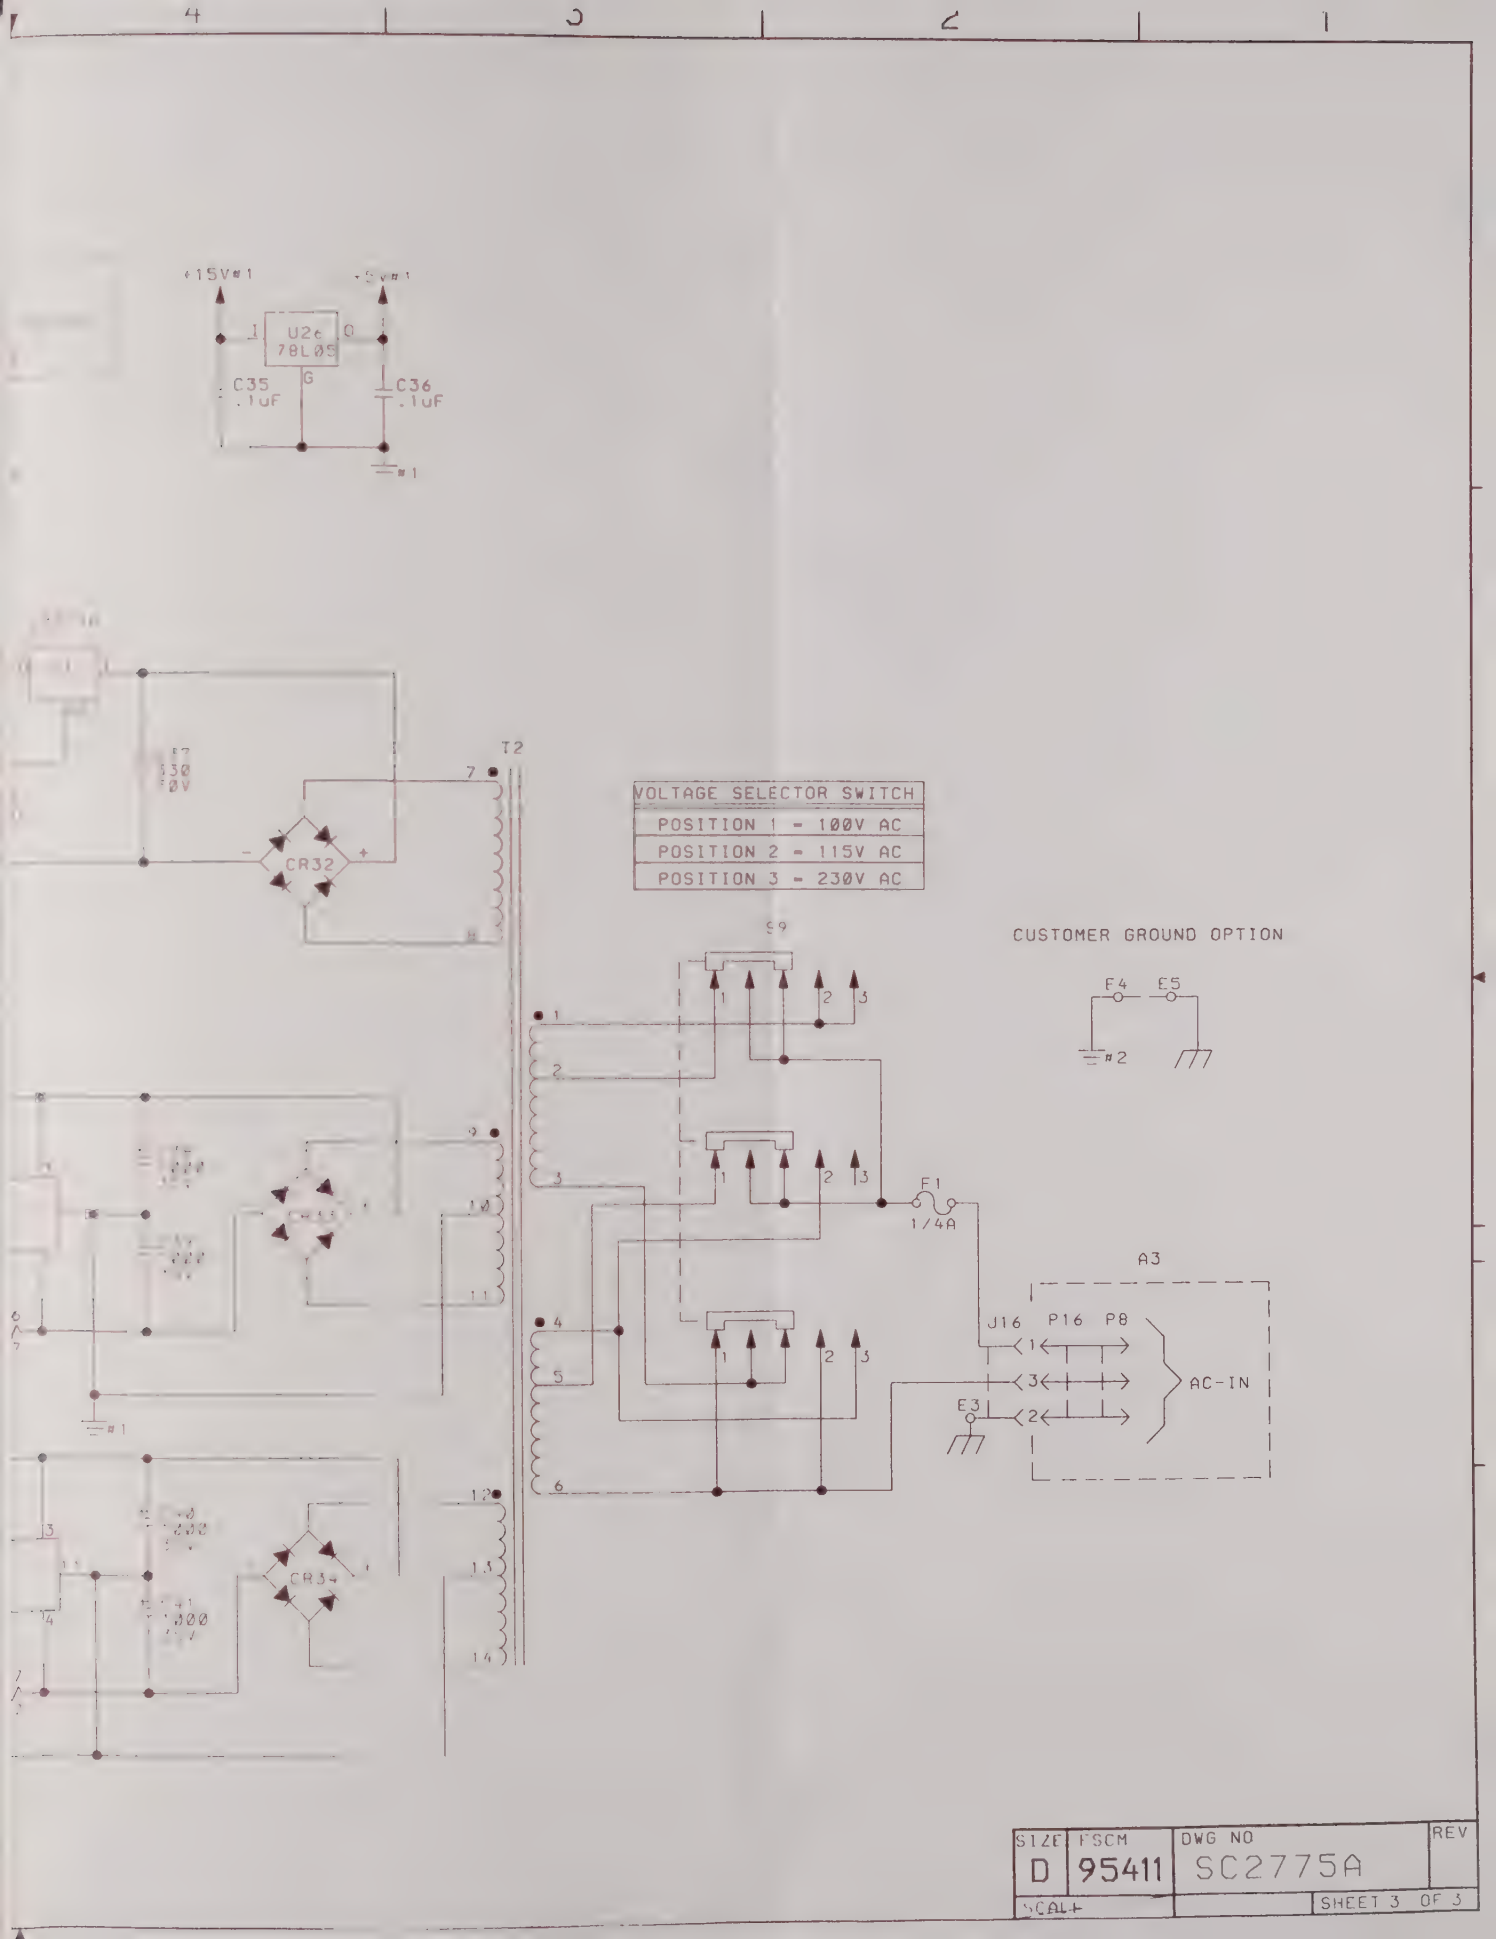

VOLTAGE SELECTOR SWITCH
POSITION 1 - 100V AC
POSITION 2 - 115V AC
POSITION 3 - 230V AC

SIZE	FSCM	DWG NO	REV
D	95411	SC2775A	
SCALE			SHEET 3 OF 3

LIST OF MATERIALS		
PART NO.	DESCRIPTION	QTY
4948	RACK	1
14769	HARDWARE MOUNTING KIT	1
16678	BLANK PANEL ASSEMBLY, SINGLE	OPT
19548	BLANK PANEL ASSY., DOUBLE	OPT

CHG	E.O.	CHANGE DESCRIPTION	BY DATE	CHK	APPR
1	7618	RELEASED	4/4/71	4/4/71	4/4/71
2	9322	ADDED P/N 19548 TO L/M DELETED "FUTURE CHG" NOTE ADDED "PRODUCT IMPROVEMENT" NOTE	11/4/71	11/5/71	11/5/71

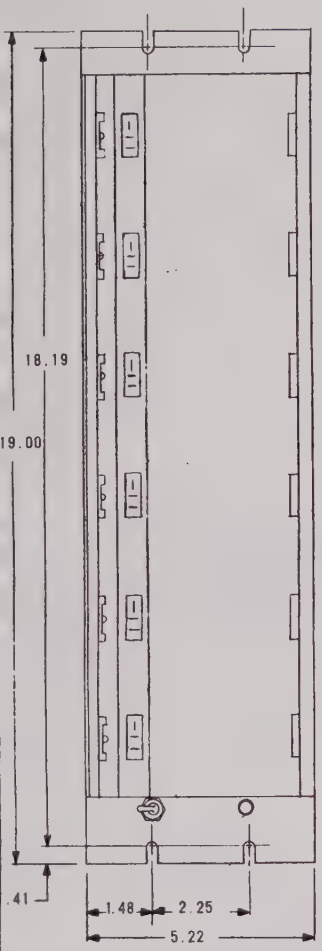

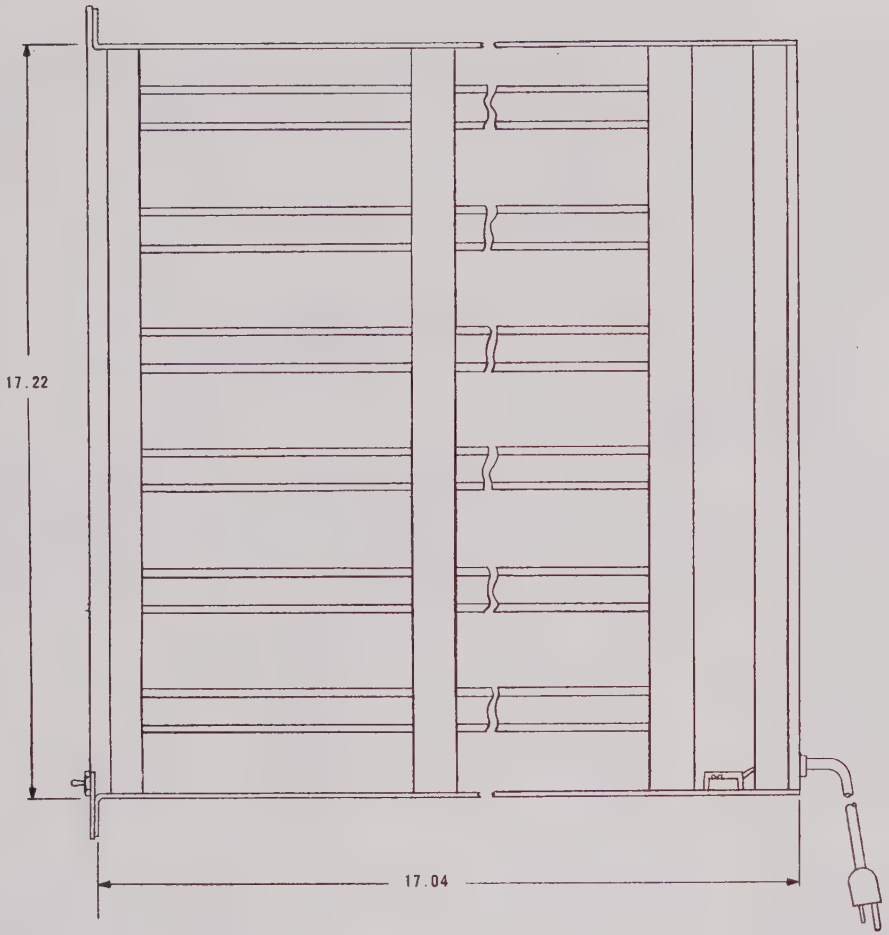

C-4948-C | 2

NOTES:

(1) SIX MODEL 6630 SIGNAL CONDITIONERS WILL FIT IN INSTRUMENT RACK MODEL 4948.

(2) FOR 230V USE, POWER CORD IS PIGTAILED AND MODEL NUMBER IS 4948V.

CONTINUED PRODUCT IMPROVEMENT NECESSITATES THAT ENDEVCO RESERVE THE RIGHT TO MODIFY THESE SPECIFICATIONS WITHOUT NOTICE TO INCORPORATE PREVIOUS ISSUES.

ENDEVCO Pasadena, California
Division of Becton, Dickinson and Company B-D

FSC 95411
DO NOT SCALE DRAWING

SPECIFICATIONS UNLESS OTHERWISE NOTED

LIMITS OF DIMS.
ANGULAR ±
FRACTIONAL ±
DECIMAL ±

1. BREAK ALL SHARP EDGES .005 MAX.
2. SURFACE ROUGHNESS 63 MICROINCH RMS MAX.
3. DIAMETERS TO BE CONCENTRIC WITHIN .005 T. I. R.
4. HOLE TOLERANCE PER AND 10387
5. ALL DIMENSIONS IN INCHES
6. FILLET RADIUS .010 MAX.

SCALE: 1/2

MATERIAL: LISTED
FINISH: —

DRAWN BY: RC 12-23-70
CHKD BY: [illegible] 3-2-71
PROJ. ENG: [illegible] 3-4-71

PART NAME: RACK

PRODUCT

SIZE C | DWG. NO. 4948-C | CHG 2

7/68 DIETERICH-POST CLEARPRINT 1000H-10

B-4948-501C A

CHG	E.O.	CHANGE DESCRIPTION	BY DATE	CHK	APPR
1	7618	RELEASED	MS 12/4/70	[illegible] 12/4/70	[illegible] 12/4/70
1A	7919	ADDED NOMENCLATURE TO POWER CONNECTOR & ADDED NOTE 3.	6/8/71	[illegible]	[illegible] 6/14/71
2	8115	REVERSED WHT & BLK PWR. LEADS	11/5/71	[illegible] 11/8/71	[illegible] 11/8/71
A	15718	ADDED CHASSIS GND AND NOTE 4	2/18/72	[illegible] 2/18/72	RK

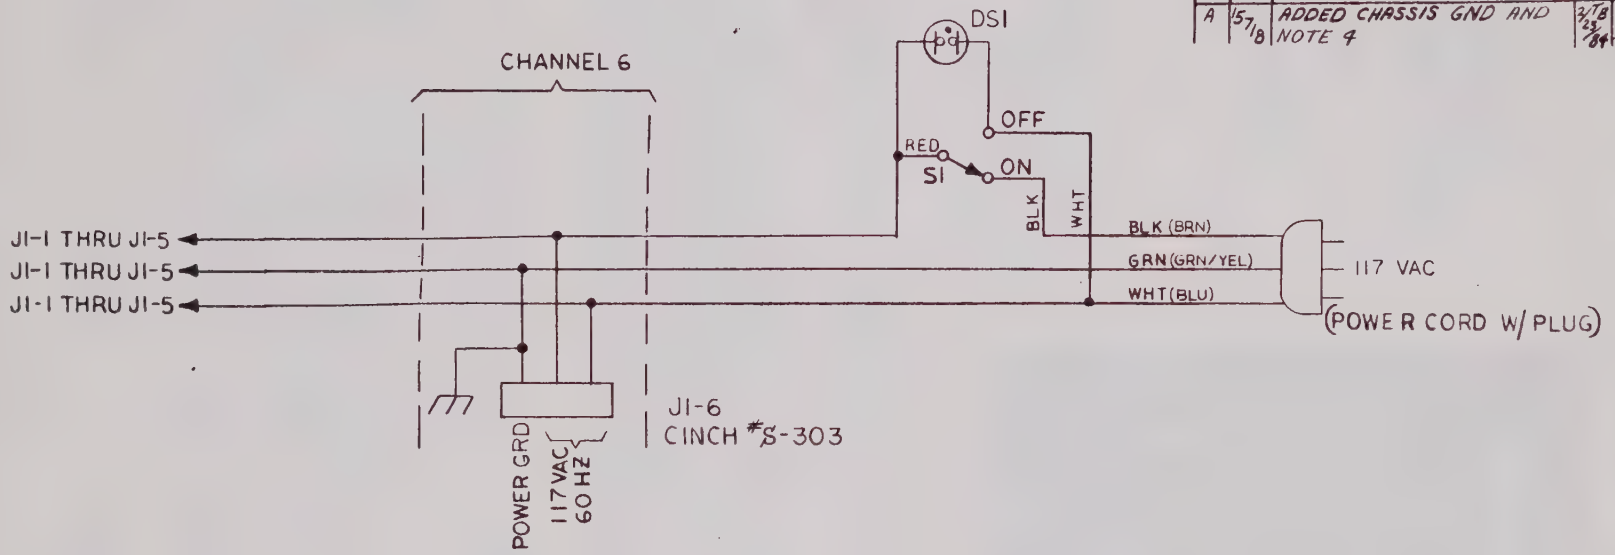

NOTES:

1 THIS DRAWING SUBJECT TO FUTURE CHANGE WITHOUT NOTICE.
2 ONE OF 6 TYPICAL CIRCUITS SHOWN.
3 FOR 230 VOLT OPERATION, MODEL-SERIAL PLATE WILL CARRY 4948V & POWER CORD WILL BE PIG TAILED.
4 WIRE COLORS IN PARENTHESES ARE INTERNATIONAL COLOR CODE.

ENDEVCO Pasadena, California
Division of Becton, Dickinson and Company B-D

FSC 5341 1

DO NOT SCALE DRAWING

SPECIFICATIONS UNLESS OTHERWISE NOTED

LIMITS OF DIMS.	
ANGULAR	± —
FRACTIONAL	± —
DECIMAL	± —

1. BREAK ALL SHARP EDGES .005 MAX.
2. SURFACE ROUGHNESS 63 MICROINCH RMS MAX.
3. DIAMETERS TO BE CONCENTRIC WITHIN .005 T. I. R.
4. HOLE TOLERANCE PER AND 10387
5. ALL DIMENSIONS IN INCHES
6. FILLET RADIUS .010 MAX.

SCALE: —

MATERIAL: —

FINISH: —

DRAWN BY: EET 12/17/70
CHKD BY: [illegible] 3-2-71
PROJ. ENG: [illegible] 3-2-71

4248V
4948
PRODUCT

PART NAME: SCHEMATIC, RACK ADAPTER

SIZE B | DWG. NO. 4948-501C | CHG 1A

IMPORTANT NOTICE: INFORMATION DISCLOSED BY THIS DRAWING IS ENDEVCO CONFIDENTIAL. REPRODUCTION, DUPLICATION, OR MANUFACTURING RIGHTS GRANTED BY WRITTEN PERMISSION ONLY.

5/70 DIETERICH-POST CLEARPRINT 1000H-10

Signal Conditioner

ENDEVCO MODEL 2775A

Model 2775A

- Multi-use, Wide Dynamic Range, Low Noise Signal Conditioner
- PE, ISOTRON® and Remote Charge Convertor Inputs
- AC, Servo and DC Outputs
- Isolated Input
- Optional Filter or Integrator

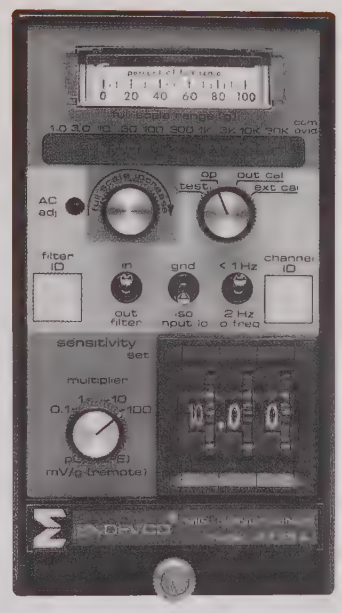

Not actual size

DESCRIPTION

The ENDEVCO® Model 2775A general purpose signal conditioner is easy to use and provides the flexibility for a wide range of testing applications. The front panel displays the settings and status of the unit. The unit provides system features of external calibration, output calibration and end-to-end testing.

The Model 2775A provides conditioning for two types of input signals: The standard PE input is compatible with a wide range of accelerometers covering the range of 0.1 to 1099 pC/g. The constant current (0.5 to 20 mA) excitation allows the 2775A to accept signals from ISOTRON (integral electronic) transducers and remote charge convertor preamplifiers.

The Model 2775A provides three standard outputs: The AC output is front panel adjustable from 1 - 10 V pk Full Scale with 85 mA current to drive large capacitive loads. The servo output provides 10 or 100 mV/g pk selectable by an internal jumper. The DC output provides a 10 VDC full scale output to drive X-Y plotters, strip chart recorders, etc. A front panel meter is provided to display percent of full scale, and is driven by the DC output. All outputs are buffered and short circuit protected. The Model 35771 plug-in filter card provides two pole Butterworth filtering in low pass or band pass configuration. The ENDEVCO Model 35818 integrator plug-in card provides velocity and displacement outputs.

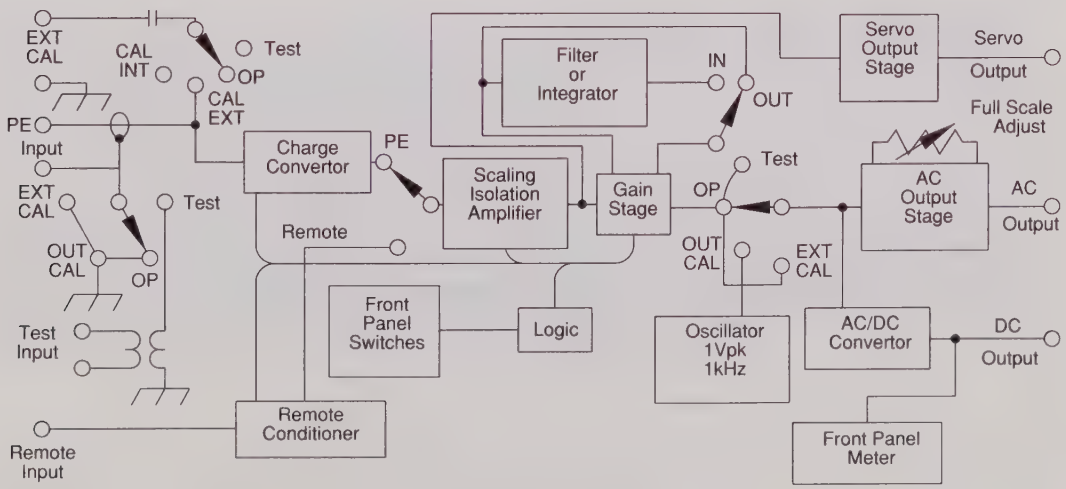

Endevco Corporation
30700 Rancho Viejo Road
San Juan Capistrano, CA 92675
(714) 493-8181 FAX (714) 661-7231

ENDEVCO MODEL 2775A

Signal Conditioner

SPECIFICATIONS

INPUTS

PIEZOELECTRIC (PE) INPUT	Single-ended with one side connected to input common
Input Charge	3000 to 110 000 pC maximum depending on gain for instantaneous recovery
Source Resistance	10 MΩ minimum
Source Capacitance	30 000 pF maximum
ISOTRON INPUT	Single-ended with one side connected to input common. Compatible with constant current systems using 2 wire remote charge convertors, or integral electronic transducers
Constant Current Excitation Supply	Adjustable from 0.5 to 20 mA DC with control located on main circuit board, factory set at 4 mA
Compliance Voltage	21 V maximum (AC + DC components)
GROUNDED INPUT MODE	The input common is connected to output common
ISOLATED INPUT MODE	The input common is isolated from output common by 50 MΩ minimum resistance in shunt with 600 pF maximum capacitance
Common Mode Voltage	6 V pk maximum to meet all specifications 500 V pk absolute maximum without damage
Maximum Common Mode Sensitivity	400 Hz to 1000 Hz, 0.025 pC/V RTI or 0.25% of F.S. per volt RTO, whichever is greater. 5 Hz to 399 Hz, 0.02 pC/V RTI or 0.1% of F.S. per volt RTO, whichever is greater.
Long Term Specification (6 months w/o adjustment)	5 Hz to 1000 Hz, 1pC/V RTI or 1.0% of Full Scale RTO, whichever is greater.
TEST INPUT	This input allows the insertion of a signal in series (transformer coupled) with the cable and the PE transducer. The signal level may be any voltage which will give a convenient reading at the output. The test frequency must be between 100 and 10 000 Hz
EXTERNAL CALIBRATION INPUT	An external calibration signal may be applied to the charge converter input through an internal capacitor of 1000 pF ± 0.5%
Input Voltage Level	To obtain F.S. output, the voltage input in mV should be Vin[mV] = FS x S where FS is the full scale setting and S is the sensitivity setting

OUTPUTS: All outputs are short-circuit protected, single-ended with one side connected to output common .

AC OUTPUT	
Full Scale Voltage	1 V pk to 10 V pk adjustable. Linear to 12 V pk. Factory set at 10 V pk.
Output Current	85 mA pk maximum
Output DC Offset	20 mV maximum, < 5 mV typical
DC OUTPUT	This output is proportional to the peak average of the AC output signal
Full Scale Output Voltage	10 VDC
Output Current	3 mA DC maximum
Output Offset Voltage	30 mV DC maximum < 5 mV DC typical
SERVO OUTPUT	
Output Sensitivity	Internally selectable 10 mV/g, 100 mV/g
Linear Output	12 V pk maximum from 1 Hz to 20 KHz
Output Current	3 mA pk maximum over specified frequency range
DC Offset	17 mV maximum, <5 mV typical

TRANSFER CHARACTERISTICS

GAIN RANGE	.03 to 1000
GAIN ACCURACY	
Input to AC, DC or Servo Output	± 1.5% of F.S. maximum, with filter disabled
Input to Meter	± 3% of F.S. maximum, with filter disabled
NOISE	PE input open circuit, a 250 Ω resistor is connected to the remote input and the current adjustment set to 4mA
PE Input/AC Output Noise	0.015 pC maximum rms plus 0.0015 pC rms per 1000 pF of source capacitance RTI or 1 mV rms RTO, whichever is greater
PE Input/ AC Output Low Frequency Noise	Less than 15 mV pk-pk RTO with 100 mV/pC gain, from 0.01 Hz to 100 Hz
Remote Input/AC Output Noise	

Full Scale	1	3	10	30	100	300	1k	3k	10k	30k
Noise mV rms	5.0	2.0	5.0	2.0	5.0	0.7	0.7	0.5	0.5	0.5

Meter Deflection (Independent of input type)	1% maximum
Servo Output (Independent of input type)	10 mV/g servo output sensitivity setting

Sensitivity Multiplier	0.1	1	10	100
Noise mV rms	20	2	0.3	0.2

TRANSFER CHARACTERISTICS–continued

FULL SCALE RANGES

Sensitivity Multiplier	Full Scale Ranges, g pk					
0.1	100	300	1k	3k	10k	30k
1	10	30	100	300	1k	3k
10	1	3	10	30	100	300
100	1	3	10	30		

FREQUENCY RESPONSE

The gain is flat within its bandwidth. At the lower and upper cutoff frequency the gain is 5% lower than the gain at 1 kHz.

Piezoelectric Mode

Lower Cutoff Frequency, AC and DC Outputs

Low frequency switch set at < 0.5 Hz — 0.5 Hz ± 0.1 Hz, -3 dB at 0.2 Hz maximum

Low frequency switch set at 2 Hz — 2.1 Hz ± 0.5 Hz, -3 dB at 0.5 Hz maximum

Upper Cutoff Frequency, AC and DC Outputs

The upper cutoff frequency depends on the full scale setting as follows:

Full Scale	1	3	10	30	100	300	1k	3k	10k	30k
-5% f [kHz] minimum	25	30	25	30	40	30	50	50	50	50

Remote Mode

Independent of low frequency switch position

Lower Cuttoff Frequency, AC and DC Outputs

-5% at 0.5 Hz maximum

-3 dB at 0.2 Hz maximum

Upper Cutoff Frequency, AC and DC Outputs

The upper cutoff frequency depends on the full scale setting as follows:

Full Scale	1	3	10	30	100	300	1k	3k	10k	30k
-5% f [kHz] minimum	24	24	24	24	30	35	70	70	70	70

AMPLITUDE LINEARITY

Input to All Outputs — 1% of reading from best fit straight line approximation

Input to Meter — ± 3% of full scale from best fit straight line from 0 to full scale

OUTPUT CALIBRATION MODE — This mode is selected from the front panel switch. A calibration voltage is provided at the AC and DC outputs. The amplitude represents 100% of full scale, regardless of range or sensitivity control settings.

Voltage Accuracy — ± 1% of full scale

Frequency — 1000 Hz ± 5%

ENVIRONMENTAL

TEMPERATURE RANGE — Operating 36°F to 125°F (2°C to 52°C); Storage -65°F to 185°F (-54°C to 85°C)

HUMIDITY — 95% R.H. maximum

POWER

INPUT VOLTAGE — Selectable through a switch located on the main board

90 - 110 V rms

105 - 125 V rms

210 - 250 V rms

FREQUENCY RANGE — 40 to 400 Hz

CURRENT — 100 mA rms maximum at 115 V rms, 60 Hz

PHYSICAL

DIMENSIONS — 4.88" h x 2.71" w x 15.81" d (12.4cm x 6.9cm x 40.2cm)

WEIGHT — 4.5 lbs (2.1 kg)

CONNECTORS — PE input: 10 - 32 Microdot®; Remote input and outputs: BNC, UG 1094/U or equivalent

ACCESSORIES

17180	Power Cord (17180V for 230 V operation)
EJ21	BNC to Microdot Connector Adapter
IM2775A	Instruction Manual

OPTIONAL ACCESSORIES

35771	Filter Card
35818	Integrator Card
4948	Rack Adapter (1 per 6 each Model 2775A/2775AM4)
16678	Blank Panel

ENDEVCO MODEL 2775A

Signal Conditioner

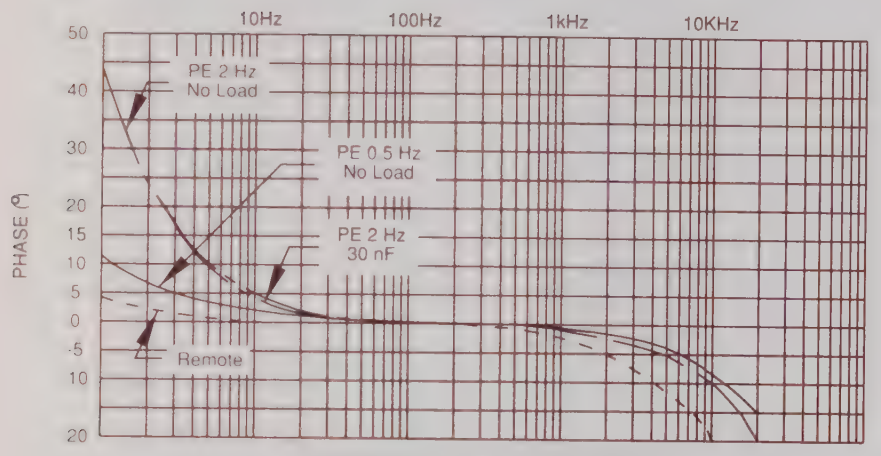

TYPICAL PHASE SHIFT VS FREQUENCY
(S=1, FS=100, AC OUTPUT)

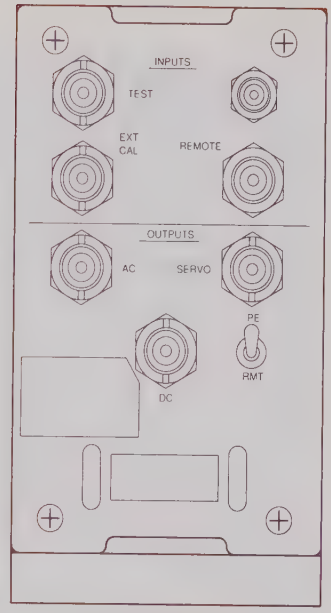

REAR PANEL

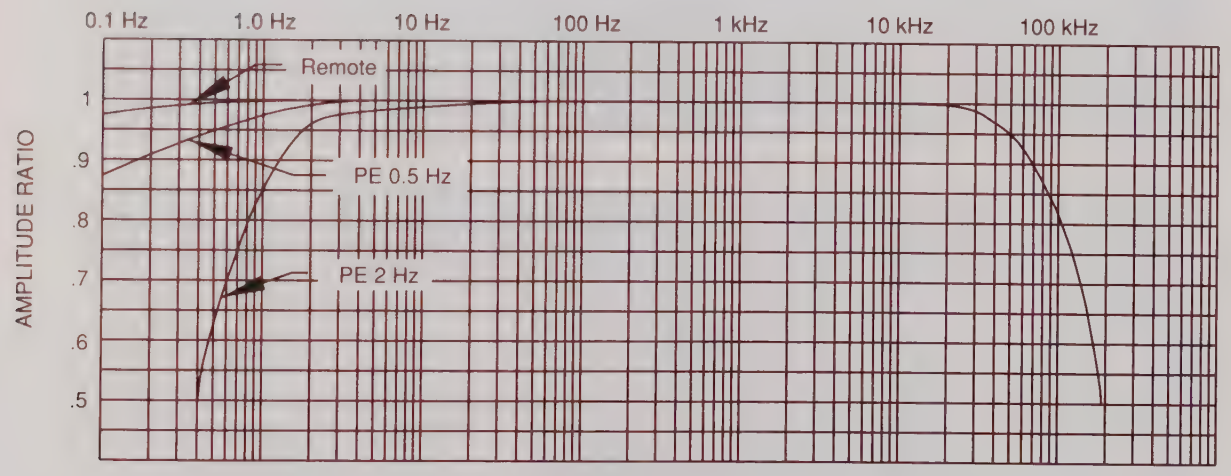

TYPICAL FREQUENCY RESPONSE
(S=1, FS=100, GAIN NORMALIZED AT 1 kHz, AC OUTPUT)

Continued product improvement necessitates that Endevco® reserve the right to modify these specifications without notice. Endevco maintains a program of constant surveillance over all products to ensure a high level of reliability. This program includes attention to reliability factors during product design, the support of stringent Quality Control requirements, and compulsory corrective action procedures. These measures, together with conservative specifications have made the name Endevco synonymous with reliability.

ENDEVCO CORPORATION, 30700 RANCHO VIEJO ROAD, SAN JUAN CAPISTRANO, CA 92675 USA (714) 493-8181 FAX (714) 661-7231

ENDEVCO® OFFICES WORLDWIDE

CORPORATE OFFICE AND PLANT
San Juan Capistrano, CA 92675
30700 Rancho Viejo Road
Telephone (714) 493-8181
Fax (714) 661-7231
Telex 685608

Alabama

W.A. Brown Instruments
1580 Sparkman Drive, Suite 106
Huntsville, Alabama 35816
Phone: (205) 830-9224
Fax: (205) 830-4371

California

Endevco
1849 Old Bayshore Highway, Suite 304A
Burlingame, California 94010
Phone: (415) 697-9887
Fax: (415) 697-1254

Endevco
1573 Ocean Front
San Diego, California 92107
Phone: (619) 222-4760
Fax: (619) 222-4412

Connetieut

Endevco
20 Holmes Street
Mystic, Connecticut 06355
Phone: (203) 572-0571
Fax: (203) 535-0439

Florida

W.A. Brown Instruments
7200 Griffin Road, Suite 3-A
Davie, Florida 33314
Phone: (305) 581-6444
Fax: (305) 581-6446

Endevco
1421 E. First Avenue
Mt. Dora, Florida 32757
Phone: (904) 383-0477
Fax: (904) 383-6558

Georgia

W.A. Brown Instruments
3850 Holcomb Bridge Road, Suite 406
Norcross, Georgia 30092
Phone: (404) 449-7160
Fax: (404) 263-7663

Illinois

Endevco
390 E. Devon
Roselle, Illinois 60172
Phone: (708) 810-9222
Fax: (708) 980-4122

Indiana

R.D.P. Corporation
PAC Plaza, Suite B-105
2346 S. Lynhurst Drive
Indianapolis, Indiana 46241
Phone: (317) 243-8788
Fax: (317) 243-8789

Maryland

Endevco
198 West Street
Annapolis, Maryland 21401
Phone: (410) 269-8800
Fax: (410) 268-5676

Michigan

R.D.P. Corporation
34600 Grand River Avenue
Farmington Hills, Michigan 48335
Phone: (313) 471-0685
Fax: (313) 471-7407

New Mexico

Endevco
9004 Menaul NE, Suite 20
Albuquerque, New Mexico 87112
Phone: (505) 292-8990
Fax: (505) 298-4799

North Carolina

W.A. Brown Instruments
106-C Fountain Brook Circle
Cary, North Carolina 27511
Phone: (919) 460-1120
Fax: (919) 469-5217

Ohio

R.D.P. Corporation
P.O. Box 470606
Cleveland, Ohio 44147
Phone: (216) 659-3138
Fax: (216) 659-6969

R.D.P. Corporation
5877 Huberville Avenue
Dayton, Ohio 45431
Phone: (513) 253-6175
Fax: (513) 254-1951

Pennsylvania

Endevco
1109 Saunders Court, Office #4
West Chester, Pennsylvania 19380
Phone: (215) 430-7024
Fax: (215) 430-0514

Washington

Endevco
310 3rd Avenue NE, Suite 101
Issaquah, Washington 98027
Phone: (206) 641-3495
Fax: (206) 392-8973

INTERNATIONAL

ENDEVCO FRANCE S.A.
23, Rue Baudin
93315 Le Pre' Saint Gervais Cedex
Phone: 011-33-1-4891-8047
Telex: 842233020
Fax: 011-33-1-4843-4526

ENDEVCO GERMANY
Geschaeftsbereich Der Allied GMBH
(Deutschland)
Schloss Wolfsbrunnenweg 15
D-6900 Heidelberg, Germany
Phone: 011-49-6221-166073
Telex: 841461605
Fax: 011-49-6221-166278

ENDEVCO UNITED KINGDOM
Melbourn, Royston, Herts
SG8 6AQ, England
Phone: 011-44-763-261311
Telex: 85181522
Fax: 011-44-763-261120

MEGGITT
AEROSPACE

ENDEVCO

30700 Rancho Viejo Road
San Juan Capistrano
California
92675
USA
telephone
(714) 493-8181
fax
(714) 661-7231
telex
68-5608 ENDEVCO SJUC

www.manualsplus.com

1028642

SE Laboratories
LOC. FF3
MAN – 06330